

Manual of Petroleum Measurement Standards Chapter 10.3

Standard Test Method for Water and Sediment in Crude Oil by the Centrifuge Method (Laboratory Procedure)

FOURTH EDITION, AUGUST 2013



AMERICAN PETROLEUM INSTITUTE

Special Notes

API publications necessarily address problems of a general nature. With respect to particular circumstances, local, state, and federal laws and regulations should be reviewed.

Neither API nor any of API's employees, subcontractors, consultants, committees, or other assignees make any warranty or representation, either express or implied, with respect to the accuracy, completeness, or usefulness of the information contained herein, or assume any liability or responsibility for any use, or the results of such use, of any information or process disclosed in this publication. Neither API nor any of API's employees, subcontractors, consultants, or other assignees represent that use of this publication would not infringe upon privately owned rights.

API publications may be used by anyone desiring to do so. Every effort has been made by the Institute to assure the accuracy and reliability of the data contained in them; however, the Institute makes no representation, warranty, or guarantee in connection with this publication and hereby expressly disclaims any liability or responsibility for loss or damage resulting from its use or for the violation of any authorities having jurisdiction with which this publication may conflict.

API publications are published to facilitate the broad availability of proven, sound engineering and operating practices. These publications are not intended to obviate the need for applying sound engineering judgment regarding when and where these publications should be utilized. The formulation and publication of API publications is not intended in any way to inhibit anyone from using any other practices.

Any manufacturer marking equipment or materials in conformance with the marking requirements of an API standard is solely responsible for complying with all the applicable requirements of that standard. API does not represent, warrant, or guarantee that such products do in fact conform to the applicable API standard.

Users of this Standard should not rely exclusively on the information contained in this document. Sound business, scientific, engineering, and safety judgment should be used in employing the information contained herein.

Where applicable, authorities having jurisdiction should be consulted.

Work sites and equipment operations may differ. Users are solely responsible for assessing their specific equipment and premises in determining the appropriateness of applying the instructions. At all times users should employ sound business, scientific, engineering, and judgment safety when using this Standard.

API is not undertaking to meet the duties of employers, manufacturers, or suppliers to warn and properly train and equip their employees, and others exposed, concerning health and safety risks and precautions, nor undertaking their obligations to comply with authorities having jurisdiction.

Information concerning safety and health risks and proper precautions with respect to particular materials and conditions should be obtained from the employer, the manufacturer or supplier of that material, or the material safety data sheet.

All rights reserved. No part of this work may be reproduced, translated, stored in a retrieval system, or transmitted by any means, electronic, mechanical, photocopying, recording, or otherwise, without prior written permission from the publisher. Contact the Publisher, API Publishing Services, 1220 L Street, NW, Washington, DC 20005.

Foreword

Nothing contained in any API publication is to be construed as granting any right, by implication or otherwise, for the manufacture, sale, or use of any method, apparatus, or product covered by letters patent. Neither should anything contained in the publication be construed as insuring anyone against liability for infringement of letters patent.

Shall: As used in a standard, "shall" denotes a minimum requirement in order to conform to the specification.

Should: As used in a standard, "should" denotes a recommendation or that which is advised but not required in order to conform to the specification.

This document was produced under API standardization procedures that ensure appropriate notification and participation in the developmental process and is designated as an API standard. Questions concerning the interpretation of the content of this publication or comments and questions concerning the procedures under which this publication was developed should be directed in writing to the Director of Standards, American Petroleum Institute, 1220 L Street, NW, Washington, DC 20005. Requests for permission to reproduce or translate all or any part of the material published herein should also be addressed to the director.

Generally, API standards are reviewed and revised, reaffirmed, or withdrawn at least every five years. A one-time extension of up to two years may be added to this review cycle. Status of the publication can be ascertained from the API Standards Department, telephone (202) 682-8000. A catalog of API publications and materials is published annually by API, 1220 L Street, NW, Washington, DC 20005.

Suggested revisions are invited and should be submitted to the Standards Department, API, 1220 L Street, NW, Washington, DC 20005, standards@api.org.

Contents

	Page
1 Scope	1
2 Referenced Documents	1
3 Summary of Test Method	2
4 Significance and Use	2
5 Apparatus	2
6 Solvent	3
7 Sampling	3
8 Procedure	3
9 Calculation	5
10 Precision and Bias	5
11 Keywords	5
Annex A1 (Mandatory Information) Procedure to Water-saturate Toulene	6
Appendix X1 (Nonmandatory Information) Precision and Accuracy of Methods for Determining Water in Crude Oils	7
Summary of Changes	13
Figures	
1 Eight-Inch (203-mm) Centrifuge Tube	3
2 Procedure for Reading Water and Sediment When Using an ASTM 100-mm Cone-Shaped Centrifuge Tube	4
3 Basic Sediment and Water Precision	5
A1.1 Solubility of Water in Toluene	6
X1.1 Basic Sediment and Water Precision for ASTM Test Method D95 (API <i>MPMS</i> Chapter 10.5) Distillation (Based on Seven Laboratories)	11
X1.2 Basic Sediment and Water Precision for ASTM Test Method D1796 (API <i>MPMS</i> Chapter 10.6) Centrifuge (Based on Five Laboratories)	12
X1.3 Basic Sediment and Water Precision for ASTM Test Method D1796 (API <i>MPMS</i> Chapter 10.6) Centrifuge (Based on Six Laboratories)	12
Tables	
1 Centrifuge Tube Calibration Tolerances for 203-mm (8-in.) Tube	3
2 Expression of Results, mL	5
X1.1 Base Case—Water Content of Crudes	7
X1.2 Water Content of Crude Oil Samples	8
X1.3 Determination of Water in Crude Oils, % H ₂ O	8
X1.4 Corrections to be Applied to Measured Values to Obtain “True” Water Content	9
X1.5 Bias of Methods Estimated from Spiked Samples	9
X1.6 Round-Robin Results of Water in Crude Oils by ASTM D95 (API <i>MPMS</i> Chapter 10.5) and ASTM D1796 (API <i>MPMS</i> Chapter 10.6)	10
X1.7 Constants	10
X1.8 ASTM Precision Intervals: ASTM D95 (API <i>MPMS</i> Chapter 10.5) (7 Laboratories)	11
X1.9 Limiting Repeatabilities and Reproducibilities	12



Standard Test Method for Water and Sediment in Crude Oil by the Centrifuge Method (Laboratory Procedure)¹

This standard is issued under the fixed designation D4007; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

^{ε1} NOTE—Referenced Documents and API information was editorially corrected in June 2013.

1. Scope*

1.1 This test method describes the laboratory determination of water and sediment in crude oils by means of the centrifuge procedure. This centrifuge method for determining water and sediment in crude oils is not entirely satisfactory. The amount of water detected is almost always lower than the actual water content. When a highly accurate value is required, the revised procedures for water by distillation, Test Method **D4006** (API *MPMS* Chapter 10.2) (**Note 1**), and sediment by extraction, Test Method **D473** (API *MPMS* Chapter 10.1), shall be used.

NOTE 1—Test Method **D4006** (API *MPMS* Chapter 10.2) has been determined to be the preferred and most accurate method for the determination of water.

1.2 The values stated in SI units are to be regarded as standard. The values given in parentheses are for information only.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use. Specific warning statements appear in 6.1, 8.3, and A1.5.4.*

2. Referenced Documents

2.1 ASTM Standards:²

D95 Test Method for Water in Petroleum Products and Bituminous Materials by Distillation (API *MPMS* Chapter 10.5)

¹ This test method is under the jurisdiction of ASTM Committee D02 on Petroleum Products and Lubricants and the API Committee on Petroleum Measurement and is the direct responsibility of Subcommittee D02.02 /COMQ on Hydrocarbon Measurement for Custody Transfer (Joint ASTM-API).

Current edition approved June 1, 2011. Published August 2011. Originally approved in 1981. Last previous edition approved in 2008 as D4007–08. DOI: 10.1520/D4007-11E01.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

D473 Test Method for Sediment in Crude Oils and Fuel Oils by the Extraction Method (API *MPMS* Chapter 10.1)
D665 Test Method for Rust-Preventing Characteristics of Inhibited Mineral Oil in the Presence of Water
D1796 Test Method for Water and Sediment in Fuel Oils by the Centrifuge Method (Laboratory Procedure) (API *MPMS* Chapter 10.6)
D4006 Test Method for Water in Crude Oil by Distillation (API *MPMS* Chapter 10.2)
D4057 Practice for Manual Sampling of Petroleum and Petroleum Products (API *MPMS* Chapter 8.1)
D4177 Practice for Automatic Sampling of Petroleum and Petroleum Products (API *MPMS* Chapter 8.2)
D4928 Test Method for Water in Crude Oils by Coulometric Karl Fischer Titration (API *MPMS* Chapter 10.9)
D5854 Practice for Mixing and Handling of Liquid Samples of Petroleum and Petroleum Products (API *MPMS* Chapter 8.3)
E969 Specification for Glass Volumetric (Transfer) Pipets
2.2 API Standards:³
MPMS Chapter 8.1 Manual Sampling of Petroleum and Petroleum Products (ASTM Practice **D4057**)
MPMS Chapter 8.2 Automatic Sampling of Petroleum and Petroleum Products (ASTM Practice **D4177**)
MPMS Chapter 8.3 Mixing and Handling of Liquid Samples of Petroleum and Petroleum Products (ASTM Practice **D5854**)
MPMS Chapter 10.1 Determination of Sediment in Crude Oils and Fuel Oils by the Extraction Method (ASTM Test Method **D473**)
MPMS Chapter 10.2 Determination of Water in Crude Oil by Distillation (ASTM Test Method **D4006**)
MPMS Chapter 10.4 Determination of Sediment and Water in Crude Oil by the Centrifuge Method (Field Procedure)
MPMS Chapter 10.5 Determination of Water in Petroleum Products and Bituminous Materials by Distillation

³ Available from American Petroleum Institute (API), 1220 L. St., NW, Washington, DC 20005-4070, www.api.org.

*A Summary of Changes section appears at the end of this standard

(ASTM Test Method D95)

MPMS Chapter 10.6 Determination of Water and Sediment in Fuel Oils by the Centrifuge Method (Laboratory Procedures) (ASTM Test Method D1796)

MPMS Chapter 10.9 Test Method for Water in Crude Oils by Coulometric Karl Fischer Titration (ASTM Test Method D4928)

2.3 *IP Standard*:⁴

Methods Book, Appendix B Specification for Methylbenzenes (Toluenes)

2.4 *ISO Standard*:⁵

ISO 5272:1979 Toluene for Industrial Use—Specifications

3. Summary of Test Method

3.1 Equal volumes of crude oil and water-saturated toluene are placed into a cone-shaped centrifuge tube. After centrifugation, the volume of the higher density water and sediment layer at the bottom of the tube is read.

4. Significance and Use

4.1 The water and sediment content of crude oil is significant because it can cause corrosion of equipment and problems in processing. A determination of water and sediment content is required to measure accurately net volumes of actual oil in sales, taxation, exchanges, and custody transfers. It is not anticipated that this test method, which is written with a dedicated laboratory facility in mind, is likely to be used in field test rooms or sample rooms due to safety concerns for proper ventilation and handling.

4.2 This test method may not be suitable for crude oils that contain alcohols that are soluble in water. In cases where the impact on the results may be significant, the user is advised to consider using another test method, such as Test Method D4928 (API MPMS Chapter 10.9).

5. Apparatus

5.1 *Centrifuge*:

5.1.1 A centrifuge capable of spinning two or more filled cone-shaped, 203-mm (8-in.) centrifuge tubes at a speed that can be controlled to give a relative centrifugal force (rcf) of a minimum of 600 at the tip of the tubes shall be used (see 5.1.6).

5.1.2 The revolving head, trunnion rings, and trunnion cups, including the cushions, shall be soundly constructed to withstand the maximum centrifugal force capable of being delivered by the power source. The trunnion cups and cushions shall firmly support the tubes when the centrifuge is in motion. The centrifuge shall be enclosed by a metal shield or case strong enough to eliminate danger if any breakage occurs.

5.1.3 The centrifuge shall be heated and controlled thermostatically to avoid unsafe conditions. It shall be capable of maintaining the sample temperature during the entire run at $60 \pm 3^\circ\text{C}$ ($140 \pm 5^\circ\text{F}$). The thermostatic control shall be capable

of maintaining the temperature within these limits and operate safely if there is a flammable atmosphere.

5.1.4 Electric powered and heated centrifuges must meet all safety requirements for use in hazardous areas.

5.1.5 Calculate the necessary minimum speed of the rotating head in revolutions per minute (r/min) as follows:

$$r/\text{min} = 1335 \sqrt{\text{rcf}/d} \quad (1)$$

where:

rcf = relative centrifugal force and

d = diameter of swing measured between tips of opposite tubes when in rotating position, mm, or

$$r/\text{min} = 265 \sqrt{\text{rcf}/d} \quad (2)$$

where:

rcf = relative centrifugal force and

d = diameter of swing measured between tips of opposite tubes when in rotating position, in.

5.1.6 Calculate the relative centrifugal force from a measured speed (r/min) as follows:

$$\text{rcf} = d \left(\frac{r/\text{min}}{1335} \right)^2 \quad (3)$$

where:

d = diameter of swing measured between tips of opposite tubes when in rotating position, mm, or

$$\text{rcf} = d \left(\frac{r/\text{min}}{265} \right)^2 \quad (4)$$

where:

d = diameter of swing measured between tips of opposite tubes when in rotating position, in.

5.2 *Centrifuge Tubes*—Each centrifuge tube shall be a 203-mm (8-in.) cone-shaped tube, conforming to dimensions given in Fig. 1 and made of thoroughly annealed glass. The graduations, numbered as shown in Fig. 1, shall be clear and distinct, and the mouth shall be constricted in shape for closure with a cork. Scale error tolerances and the smallest graduations between various calibration marks are given in Table 1 and apply to calibrations made with air-free water at 20°C (68°F), when reading the bottom of the shaded meniscus. The accuracy of the graduations on the centrifuge tube shall be volumetrically verified, before use of the tube. The verification shall include calibration at each mark up to the 0.25 mL mark (as shown in Fig. 2), and at the 0.5, 1.0, 1.5, 2.0, 50.0, and 100 mL marks. The tube shall not be used if the scale error at any mark exceeds the applicable tolerance from Table 1.

5.3 *Bath*—The bath shall be either a solid metal block bath or a liquid bath of sufficient depth for immersing the centrifuge tube in the vertical position to the 100-mL mark. Means shall be provided for maintaining the temperature at $60 \pm 3^\circ\text{C}$ ($140 \pm 5^\circ\text{F}$). For some crude oils, temperatures of $71 \pm 3^\circ\text{C}$ ($160 \pm 5^\circ\text{F}$) may be required to melt wax crystals in crude oils. For these crude oils, the test temperature shall be maintained high enough to ensure the absence of wax crystals.

⁴ Available from Energy Institute, 61 New Cavendish St., London, WIG 7AR, U.K., <http://www.energyinst.org.uk>.

⁵ Available from American National Standards Institute (ANSI), 25 W. 43rd St., 4th Floor, New York, NY 10036, <http://www.ansi.org>.

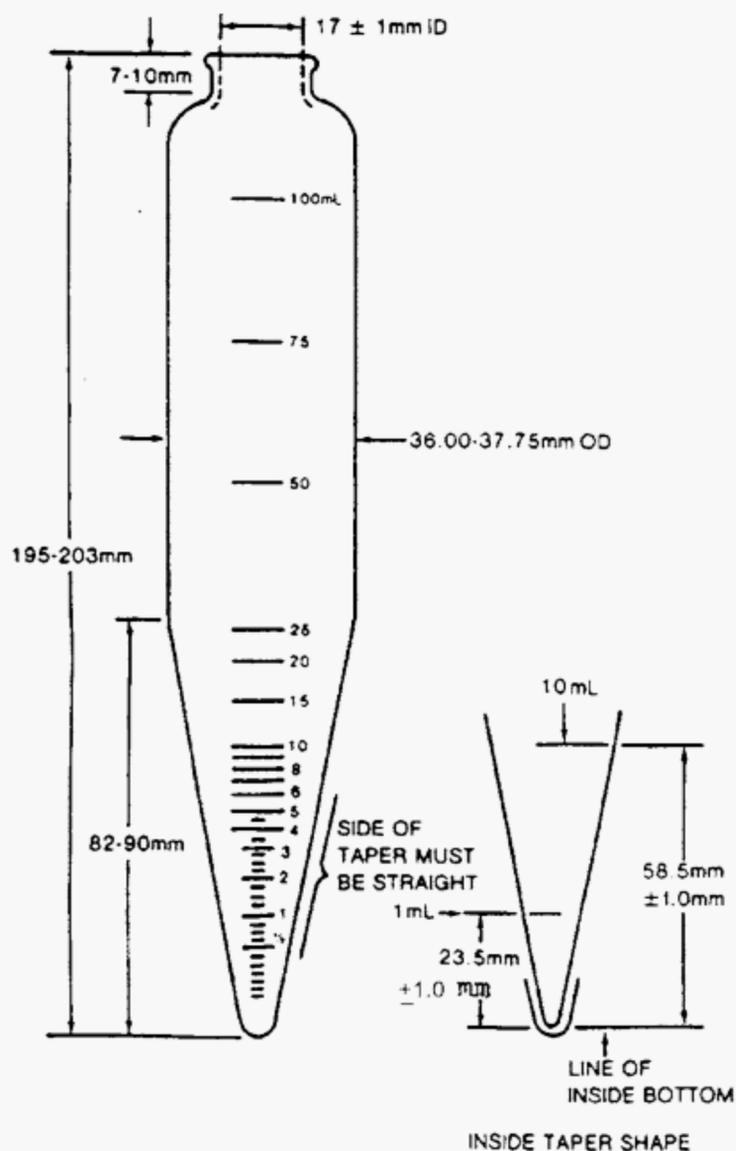


FIG. 1 Eight-Inch (203-mm) Centrifuge Tube

TABLE 1 Centrifuge Tube Calibration Tolerances for 203-mm (8-in.) Tube

Range, mL	Subdivision, mL	Volume Tolerance, mL
0 to 0.1	0.05	±0.02
Above 0.1 to 0.3	0.05	±0.03
Above 0.3 to 0.5	0.05	±0.05
Above 0.5 to 1.0	0.10	±0.05
Above 1.0 to 2.0	0.10	±0.10
Above 2.0 to 3.0	0.20	±0.10
Above 3.0 to 5.0	0.5	±0.20
Above 5.0 to 10	1.0	±0.50
Above 10 to 25	5.0	±1.00
Above 25 to 100	25.0	±1.00

5.4 50 mL Pipet, Class A, or equivalent volume dispensing device, capable of delivering a volume of 50 ± 0.05 mL (see Specification E969) for use in the test.

6. Solvent

6.1 Toluene—Reagent grade conforming to the specifications of the Committee on Analytical Reagents of the American Chemical Society (ACS)⁶ or to Grade 2 of ISO 5272 or conforming to the EI Specification for Methylbenzenes (Tolu-

⁶ Reagent Chemicals, American Chemical Society Specifications, American Chemical Society, Washington, DC. For Suggestions on the testing of reagents not listed by the American Chemical Society, see *Annual Standards for Laboratory Chemicals*, BDH Ltd., Poole, Dorset, U.K., and the *United States Pharmacopeia and National Formulary*, U.S. Pharmacopeial Convention, Inc. (USPC), Rockville, MD.

enes). (**Warning**—Flammable. Keep away from heat, sparks, and open flame. Vapor harmful. Toluene is toxic. Particular care must be taken to avoid breathing the vapor and to protect the eyes. Keep container closed. Use with adequate ventilation. Avoid prolonged or repeated contact with the skin.)

6.1.1 Typical characteristics for this reagent are:

Assay	99.5+ %
Color (APHA)	10
Boiling range (initial to dry point) (Recorded boiling point 110.6°C)	2.0°C
Residue after evaporation	0.001 % max – wt/wt
Substances darkened by H ₂ SO ₄	passes test
Sulfur compounds (as S)	0.003 % max – wt/wt
Water (H ₂ O) (by Karl Fischer titration)	0.03 % max – wt/wt

6.1.2 The solvent shall be water-saturated at $60 \pm 3^\circ\text{C}$ ($140 \pm 5^\circ\text{F}$) (see 5.3) but shall be free of suspended water. See Annex A1 for the solvent-water saturation procedure.

6.2 Demulsifier—A demulsifier should be used to promote the separation of water from the sample and to prevent its clinging to the walls of the centrifuge tube. The recommended stock solution is 25 % demulsifier to 75 % toluene. For some crude oils a different ratio of demulsifier to toluene may be required. Demulsifiers used in the concentration and quantity recommended will not add to the water and sediment volume determined. The solution must be stored in a dark bottle that is tightly closed.

7. Sampling

7.1 Sampling is defined as all steps required to obtain an aliquot of the contents of any pipe, tank, or other system and to place the sample into the laboratory test container.

7.2 Only representative samples obtained as specified in Practices D4057 (API MPMS Chapter 8.1) and Practice D4177 (API MPMS Chapter 8.2) shall be used for this test method.

7.3 Sample Mixing—is typically required to obtain a test portion representative of the bulk sample to be tested, but precautions shall be taken to maintain the integrity of the sample during this operation. Mixing of volatile crude petroleum containing water or sediments, or both, may result in the loss of light components. Additional information on the mixing and handling of liquid samples can be found in Practice D5854 (API MPMS Chapter 8.3).

8. Procedure

8.1 Fill each of two centrifuge tubes (5.2) to the 50-mL mark with sample directly from the sample container. Using a pipet or other suitable volume transfer device (see 5.4), add 50 ± 0.05 mL of toluene, which has been water saturated at 60°C (140°F) or 71°C (160°F) (see 5.3). Read the top of the meniscus at both the 50 and 100-mL marks. Add 0.2 mL of demulsifier solution (6.2) to each tube, using a 0.2-mL pipet or other suitable volume transfer device, such as an automatic pipettor. Stopper the tube tightly and invert the tubes ten times to ensure that the oil and solvent are uniformly mixed.

8.2 In the case where the crude oil is very viscous and mixing of the solvent with the oil would be difficult, the solvent may be added to the centrifuge tube first to facilitate mixing. Take care to not fill the centrifuge tube past the 100-mL mark with the sample.

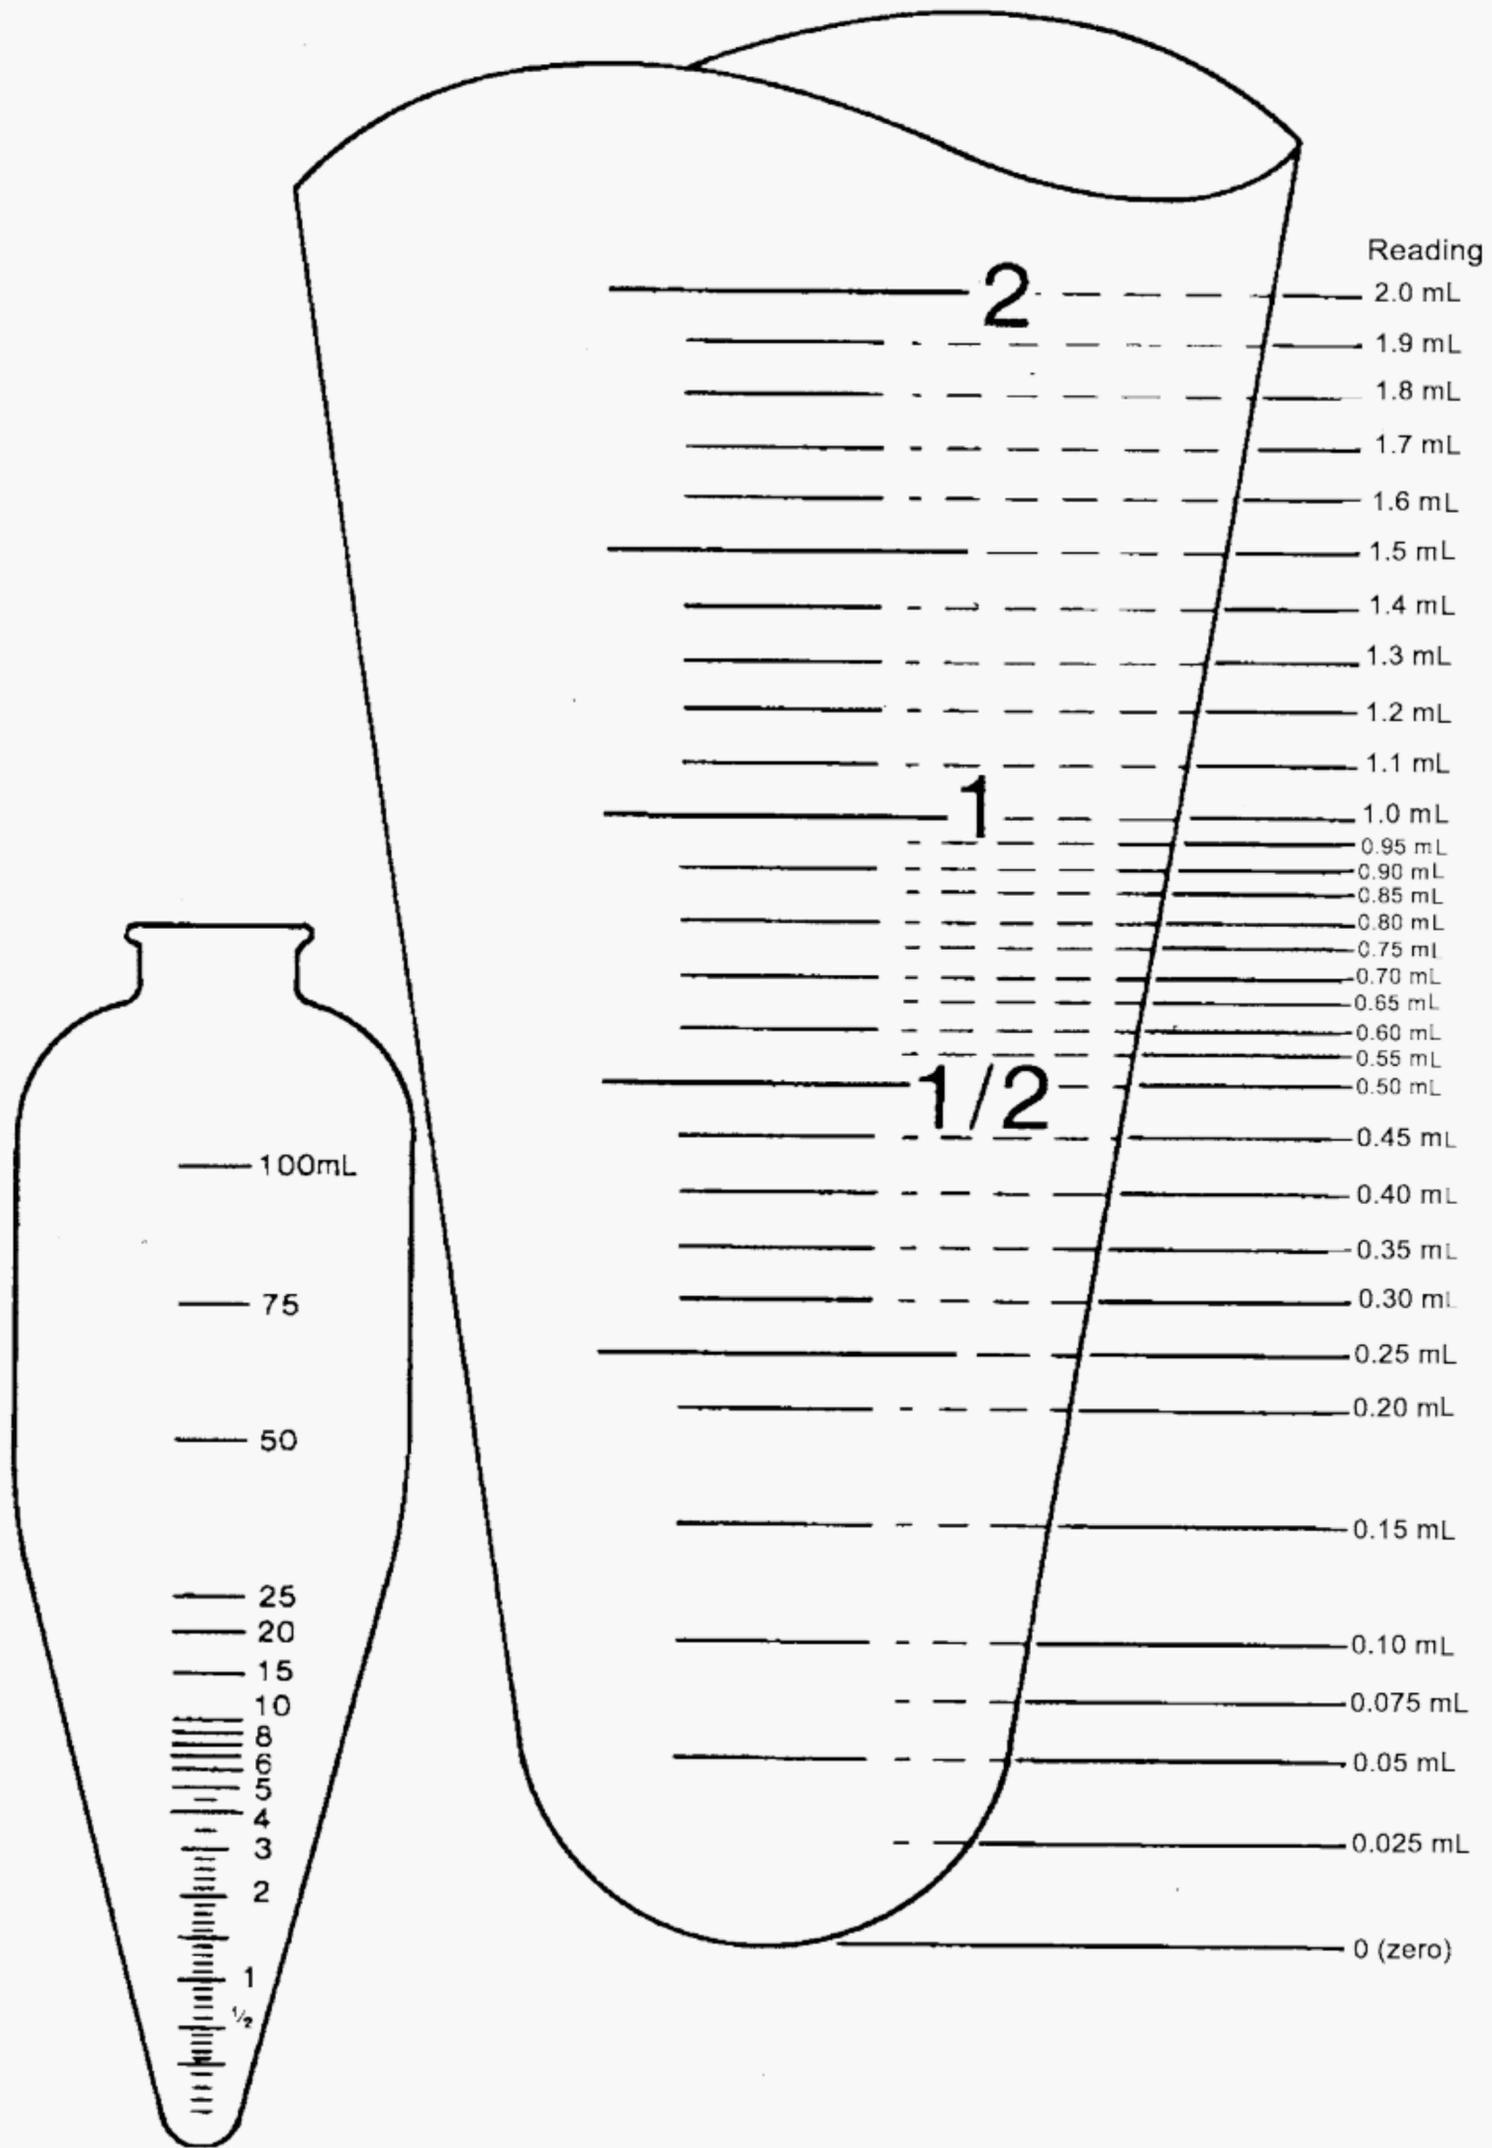


FIG. 2 Procedure for Reading Water and Sediment When Using an ASTM 100-mm Cone-Shaped Centrifuge Tube

8.3 Loosen the stoppers slightly and immerse the tubes to the 100-mL mark for at least 15 min in the bath maintained at $60 \pm 3^\circ\text{C}$ ($140 \pm 5^\circ\text{F}$) (see 5.3). Secure the stoppers and again invert the tubes ten times to ensure uniform mixing of oil and solvent. (**Warning**—The vapor pressure at 60°C (140°F) is approximately double that at 40°C (104°F .)

8.4 Place the tubes in the trunnion cups on opposite sides of the centrifuge to establish a balanced condition. (If the tubes cannot be counter-balanced by eye, place them, in their trunnion cups, on either side of a balance and equalize their masses by the addition of water to the trunnion cups.) Re-tighten the corks and spin for 10 min at a minimum relative centrifugal force of 600 calculated from the equation given in 5.1.6.

8.5 Immediately after the centrifuge comes to rest following the spin, read and record the combined volume of water and sediment at the bottom of each tube, to the nearest 0.05 mL from 0.1 to 1-mL graduations, and to the nearest 0.1-mL above 1-mL graduations. Below 0.1 mL, estimate to the nearest 0.025 mL (refer to Fig. 2). Return the tubes without agitation to the centrifuge and spin for another 10 min at the same rate.

8.6 Repeat this operation until the combined volume of water and sediment remains constant for two consecutive readings. In general, not more than two spinings are required.

8.7 The temperature of the sample during the entire centrifuging procedure shall be maintained at $60 \pm 3^\circ\text{C}$ ($140 \pm 5^\circ\text{F}$) (see 5.3).

8.8 To avoid the danger of tubes breaking in the cups, care must be taken that the tubes are bedded onto the bottom cushion so that no part of the tube is in contact with the rim of the cup.

9. Calculation

9.1 Record the final volume of water and sediment in each tube. If the difference between the two readings is greater than one subdivision on the centrifuge tube (see Table 1) or 0.025 mL for readings of 0.10 mL and below, the readings are inadmissible and the determination shall be repeated.

9.2 Express the sum of the two admissible readings as the percentage by volume of water and sediment; report the results as shown in Table 2.

TABLE 2 Expression of Results, mL

Tube 1	Tube 2	Total Percent Water and Sediment, % (V/V)
No visible water and sediment	No visible water and sediment	0.00
No visible water and sediment	0.025	0.025
0.025	0.025	0.05
0.025	0.05	0.075
0.05	0.05	0.10
0.05	0.075	0.125
0.075	0.075	0.15
0.075	0.10	0.175
0.10	0.10	0.20
0.10	0.15	0.25

10. Precision and Bias

10.1 *Precision*—The precision of this test method, as determined by statistical examination of interlaboratory test results in the range from 0.01 to 1.0 %, is described in 10.1.1 and 10.1.2.

10.1.1 *Repeatability*—The difference between two test results, obtained by the same operator with the same apparatus under constant operating conditions on identical test material, would, in the long run, in the normal and correct operation of the test method, exceed the following value in only one case in twenty:

From 0.0 % to 0.3 % water, see Fig. 3.

From 0.3 % to 1.0 % water, repeatability is constant at 0.12.

10.1.2 *Reproducibility*—The difference between two single and independent test results obtained by different operators working in different laboratories on identical test material, would, in the long run, in the normal and correct operation of the test method, exceed the following value in only one case in twenty:

From 0.0 % to 0.3 % water, see Fig. 3.

From 0.3 % to 1.0 % water, reproducibility is constant at 0.28.

10.2 *Bias*—The procedure in this test method has no bias because the value of water and sediment can be defined only in terms of a test method.

11. Keywords

11.1 centrifuge; centrifuge tube; crude oil; laboratory procedure; sampling; sediment and water; solvent

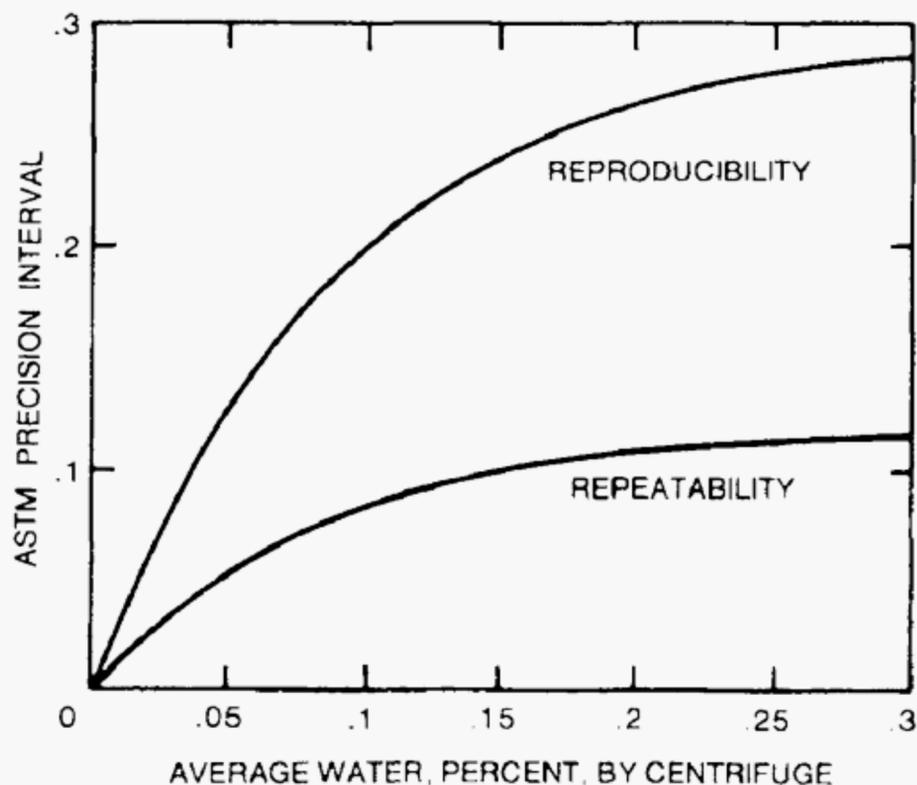


FIG. 3 Basic Sediment and Water Precision

ANNEX

(Mandatory Information)

A1. PROCEDURE TO WATER-SATURATE TOLUENE

A1.1 Scope

A1.1.1 This method is satisfactory for the water saturation of toluene to be used for determination of water and sediment in crude oils by the centrifuge method.

A1.2 Significance

A1.2.1 **Fig. A1.1** shows that water is soluble in toluene to a significant extent. The percentage of water that will dissolve increases as the temperature is increased from about 0.03 % at 21°C (70°F) to about 0.17 % at 70°C (158°F). Toluene, as normally supplied, is relatively dry and if used in an as-received condition, will dissolve a portion of or even all of any water present in a crude oil sample. This would reduce the apparent sediment and water level in the crude sample. To determine water and sediment accurately by centrifuge on a crude oil sample, the toluene must first be saturated at the centrifuge test temperature.

A1.3 Reagents

A1.3.1 *Toluene*—Reagent grade conforming to the specifications of the Committee on Analytical Reagents of the American Chemical Society (ACS)⁶ or to Grade 2 of ISO 5272, or conforming to the EI Specification for Methylbenzenes (Toluenes).

A1.3.2 *Water*, either distilled or tap water.

A1.4 Apparatus

A1.4.1 *Liquid-Heating Bath*, of sufficient depth for immersing a 1-qt or 1-L bottle to its shoulder. Means shall be provided for maintaining the temperature at $60 \pm 3^\circ\text{C}$ ($140 \pm 5^\circ\text{F}$) (see 5.3).

A1.4.2 *Glass Bottle*, 1-qt or 1-L, with screw top.

A1.5 Procedure

A1.5.1 Adjust the heating bath to the temperature at which the centrifuge test is to be run. Maintain the bath temperature to $\pm 3^\circ\text{C}$ ($\pm 5^\circ\text{F}$).

A1.5.2 Fill the glass bottle with 700 to 800 mL of toluene. Add sufficient water (at least 2 mL but not more than 25 mL) to maintain a visual indication of excess water. Screw the cap on the bottle and shake vigorously for 30 s.

A1.5.3 Loosen the cap and place the bottle in the bath for 30 min. Remove the bottle, tighten the cap, and shake cautiously for 30 s.

A1.5.4 Repeat the above procedure (A1.5.3) 3 times. (**Warning**—The vapor pressure of toluene at 60°C (140°F) is approximately twice that at 38°C (100°F).

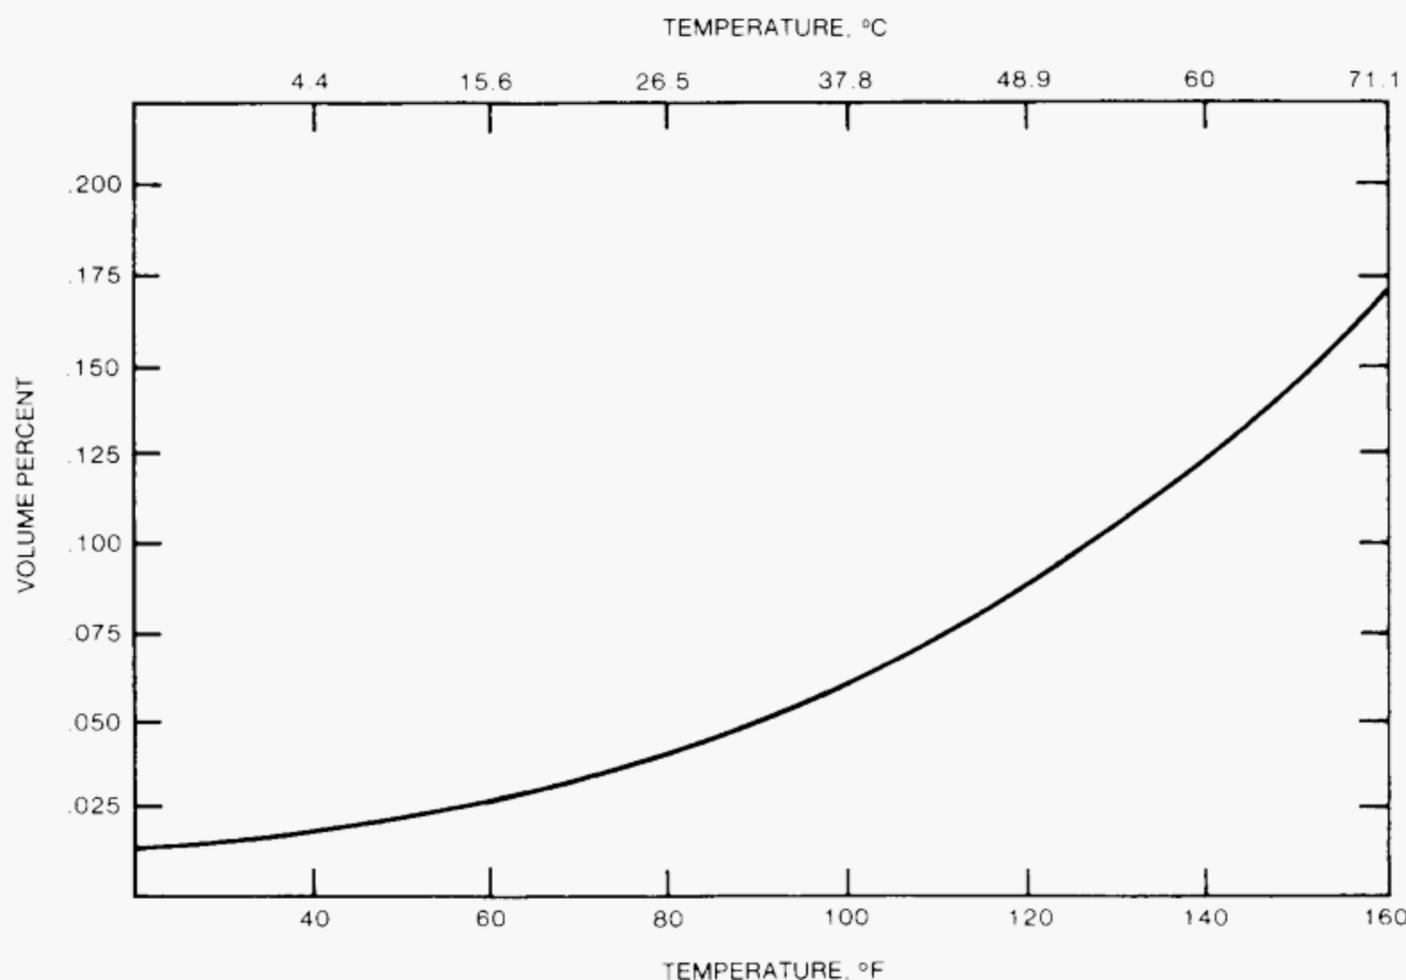


FIG. A1.1 Solubility of Water in Toluene

A1.5.5 Allow the bottle with the water-toluene mixture to sit in the bath 48 h before using. This will ensure complete equilibrium between the toluene and the free water as well as complete saturation at the desired temperature. If it is necessary to use the water-saturated toluene before the 48-h equilibration time has been completed, the solvent must be poured into centrifuge tubes and centrifuged in the same equipment at the same relative centrifuge force and temperature that is used

for the centrifuge test. The toluene must be carefully pipetted from the centrifuge tube so that any free water that may be in the bottom of the tube is not disturbed.

A1.5.6 Saturation is time- and temperature-dependent. It is recommended that bottles of the toluene-water mixture be kept at test temperature in the bath at all times so that saturated solvent will be available whenever tests are to be run.

APPENDIX

(Nonmandatory Information)

X1. PRECISION AND ACCURACY OF METHODS FOR DETERMINING WATER IN CRUDE OILS

X1.1 Summary

X1.1.1 This round-robin testing program has shown that the distillation method as practiced is somewhat more accurate than the centrifuge method. The average correction for the distillation method is about 0.06, whereas the centrifuge correction is about 0.10. However, this correction is not constant nor does it correlate well with the measured concentration.

X1.1.2 There is a slight improvement in the precision of the distillation method over the present Test Method D95 (API MPMS Chapter 10.5): 0.08 repeatability versus 0.1, and 0.11 versus 0.2 for reproducibility. These figures are applicable from 0.1 to 1 % water content, the maximum level studied in this program.

X1.1.3 The precision of the centrifuge method is worse than the distillation method: repeatability is 0.12 and the reproducibility is 0.28.

X1.2 Introduction

X1.2.1 In view of the economic importance of measuring the water content of crude oils precisely and accurately, a working group of API/ASTM Joint Subcommittee on Static Petroleum Measurement undertook the evaluation of two methods for determining water in crudes. A distillation method, Test Method D95 (API MPMS Chapter 10.5), and a centrifuge method, Test Method D1796 (API MPMS Chapter 10.6), were evaluated in this program. Both methods were modified slightly in an attempt to improve the precision and accuracy.

X1.3 Experimental Procedure

X1.3.1 *Samples*—The following seven crude oils were obtained for this program:

Crude	Source
San Ardo	Texaco
Arabian Light	Mobil
Alaskan	Williams Pipe Line
Arabian Heavy	Exxon
Minas	Texaco
Fosterton	Koch Industries
Nigerian	Gulf

By removing all water or adding known amounts of water to the above crudes, 21 samples were prepared for testing. Each

crude oil was represented at three levels of water concentration. The entire concentration range studied was from zero to 1.1 % water. These expected values were used to determine the accuracy of the test procedures.

X1.3.2 Sample Preparation:

X1.3.2.1 The crude oils were received from the suppliers in barrels. After mixing by rolling and turning, two 5-gal samples and one 250-mL sample were taken from each barrel. The Minas crude had to be heated to 150°F with a barrel heater before samples could be drawn. The 250-mL samples of each crude, as received, were used to establish the base case in water content. Each sample was analyzed by Test Method D95 (API MPMS Chapter 10.5) to determine the water content. These starting points are shown in Table X1.1.

X1.3.2.2 To obtain “water-free” samples of crude oil, one 5-gal sample of each of two crudes was distilled over the temperature range of initial to 300°F vapor temperature. This distillation was done using a 15 theoretical plate column at 1:1 reflux ratio.

X1.3.2.3 “Spiking” samples to a known water concentration was done using synthetic sea water (as described in Test Method D665). The mixing and homogenization was done with a static blender. The complete listing of samples with their expected water contents is shown in Table X1.2.

X1.3.2.4 The samples for each cooperator were bottled so that the entire sample had to be used for a given test. In this way, any effect due to settling or stratification of water was eliminated.

X1.3.2.5 Samples were coded to mask the presence of duplicates and a table of random numbers dictated the running order of tests.

X1.3.2.6 The participating laboratories were:

TABLE X1.1 Base Case—Water Content of Crudes

Crude Oil	% H ₂ O
San Ardo	0.90
Arabian Light	0.15
Alaskan	0.25
Arabian Heavy	0.10
Minas	0.50
Fosterton	0.30
Nigerian	<0.05

TABLE X1.2 Water Content of Crude Oil Samples

Crude Source	%H ₂ O		
	Found	Added	Expect
San Ardo	0.90	0	0.90
		dried	0.0
		dried + 0.4	0.40
Arabian Light	0.15	0	0.15
		0.10	0.25
		0.90	1.05
Alaskan	0.25	0	0.25
		0.20	0.45
		0.80	1.05
Arabian Heavy	0.10	0	0.10
		dried	0.0
		dried + 0.1	0.10
Minas	0.50	0	0.50
		0.10	0.60
		0.50	1.00
Fosterton	0.30	0	0.30
		0.20	0.50
		0.80	1.10
Nigerian	0.05	0	<0.05
		0.40	0.45
		0.80	0.85

Chevron Research Co.
 Exxon Research and Engineering Co.
 Mobil Research and Development Corp.
 Texaco, Inc.
 Shell
 Charles Martin, Inc.
 Gulf Research and Development Co.

X1.3.3 *Test Modifications*—The base methods studied were modified slightly in an effort to improve the performance. The modifications were as follows:

X1.3.3.1 *Test Method D95 (API MPMS Chapter 10.5)*—Sample size was standardized at 200 g and the solvent volume was increased to maintain the original solvent/sample ratio.

X1.3.3.2 *Test Method D1796 (API MPMS Chapter 10.6)*—A heated centrifuge (held near 140°F) and use of a demulsifier were mandatory. Eight-inch centrifuge tubes were also specified. Toluene saturated with water at 60°C (140°F) was the only permissible solvent. The demulsifier used was a Tret-O-Lite material, F65.⁷

X1.4 Results and Discussion

X1.4.1 Accuracy:

X1.4.1.1 Accuracy or bias is defined as the closeness of the measured value to the “true value.” Since there is no independent absolute method available to determine this true value for these samples, some other means must be used. Two options were considered:

(1) Select one laboratory and one method as the “reference system” and define these results as the true value; or

(2) Spike samples with known amounts of water. The measured difference between the original and unspiked samples can be compared to the known added water to determine the bias (accuracy). Both approaches were investigated in this study.

X1.4.1.2 Since API MPMS Chapter 10.4 defines the base method as a combination of Test Method D95 (API MPMS Chapter 10.5) and Test Method D473 (API MPMS Chapter 10.1), it was decided that data obtained by Test Method D95 (API MPMS Chapter 10.5) in one laboratory would be the “true value.” Table X1.3 shows the expected value compared to each sample average using this criterion. Both methods are biased on the low side. However, the distillation test method, Test Method D95 (API MPMS Chapter 10.5) appears less biased than the centrifuge method. Since the bias is not the same in every laboratory (Table X1.4), it is not possible to recommend inclusion of a correction factor in the methods. This data treatment suggests that the centrifuge method, on the average, yields results about 0.06 % lower than the distillation method. The respective biases are –0.13 for the centrifuge method and –0.07 for the distillation method.

X1.4.1.3 A more reliable estimate of bias may be obtained if consideration is given only to those samples to which water was added. In this case, the measured differences between the unspiked sample and the spiked sample compared to the actual water added would be indicative of the bias. Table X1.5 shows these differences for each method. On this basis the centrifuge bias has improved slightly, while the distillation method bias is about the same. The difference between the two methods is now 0.04 rather than 0.06. It should be noted that bias is greatest with both methods at higher water content.

X1.4.2 Precision:

X1.4.2.1 To estimate the precision of the tests, the data were analyzed following the ASTM guidelines published as RR:D02-1007.

X1.4.2.2 Seven laboratories participated in the round robin. Basic sediment and water was measured on 21 crude oil samples in duplicate by the distillation test method, Test Method D95 (API MPMS Chapter 10.5) and the centrifuge test method, Test Method D1796 (API MPMS Chapter 10.6). The raw data are presented in Table X1.6.

TABLE X1.3 Determination of Water in Crude Oils, % H₂O

Expected	Distillation	Centrifuge
0.90	0.90	0.79
0.0	0.04	0.05
0.40	0.42	0.021
0.15	0.10	0.12
0.25	0.21	0.13
1.05	0.86	0.78
0.25	0.21	0.14
0.45	0.39	0.32
1.05	0.92	0.98
0.10	0.11	0.04
0.0	0.06	0.02
0.10	0.18	0.10
0.50	0.45	0.34
0.60	0.53	0.47
1.00	0.96	0.97
0.30	0.18	0.07
0.50	0.33	0.20
1.10	0.86	0.77
0.05	0.02	0.01
0.45	0.35	0.32
0.85	0.65	0.65

⁷ Tret-O-Lite is a registered trademark of Tretolite Div., Petrolite Corp., 369 Marshall Ave., St. Louis, MO. Even though Tret-O-Lite F65 was used during the round robin, there are many demulsifiers on the market that may be used.

TABLE X1.4 Corrections to be Applied to Measured Values to Obtain “True” Water Content

Method	Laboratory	Correction
D1796 (API MPMS Chapter 10.6) Centrifuge	C	+ 0.152±0.095
	E	+ 0.029±0.125
	M	+ 0.196±0.135
	T	+ 0.196±0.100
	S	+ 0.160±0.122
	I	+ 0.116±0.126
	G	+ 0.121±0.115
	Average	+ 0.132
D95 (API MPMS Chapter 10.5) Distillation	C	+ 0.777±0.082
	E	+ 0.048±0.078
	M	+ 0.082±0.077
	T	+ 0.064±0.079
	S	+ 0.077±0.107
	I	+ 0.061±0.112
	G	+ 0.072±0.096
	Average	+ 0.069

TABLE X1.5 Bias of Methods Estimated from Spiked Samples

Water Added, ^A %	D95 (API MPMS Chapter 10.5)		D1796 (API MPMS Chapter 10.6)	
	Found	Δ	Found	Δ
0.10	0.10	0	0.05	-0.05
0.10	0.08	-0.02	0.00	-0.10
0.10	0.10	0	0.10	0
0.20	0.16	-0.04	0.16	-0.04
0.20	0.15	-0.05	0.12	0.00
0.40	0.39	-0.01	0.16	-0.24
0.40	0.33	-0.07	0.30	-0.10
0.50	0.49	-0.01	0.52	+ 0.02
0.80	0.70	-0.10	0.73	-0.07
0.80	0.70	-0.10	0.70	-0.10
0.80	0.64	-0.16	0.63	-0.17
0.90	0.76	-0.14	0.69	-0.21
	Average	-0.06		-0.10

^A Equal water additions shown are to different crude oils.

X1.4.3 *Test for Outliers*—Procedures for rejecting outliers recommended in ASTM RR:D02-1007, “Manual on Determining Precision Data for ASTM Methods on Petroleum Products and Lubricants,” were followed.

X1.4.3.1 *Distillation Method*—The following table lists the outliers rejected and the substituted values:

Laboratory	Sample	Rejected Value	Substituted Value
1	14	0.75	0.53
3	3	0.35, 0.54	0.445
2	11	0.34	0.06
6	13	0.66	0.45
6	15	1.37	0.85

X1.4.3.2 *Centrifuge Method*—The data from Laboratory 5 were rejected outright because incorrect-size centrifuge tubes were used (letter, Shell Oil to E. N. Davis, cc: Tom Hewitt, February 9, 1979). Statistical tests showed that Laboratory 5’s data did not belong to the same population as the other data.

(1) Laboratory 2’s data were also suspect and did not appear to belong to the same population as the other data. However, it was learned that Laboratory 2’s results were closest to actual levels of water added to the samples. There is, therefore, a dilemma on whether or not to reject Laboratory 2’s data. As a compromise, precision was calculated with and without Laboratory 2’s results. The following table lists the outliers rejected and the substituted values when Laboratory 2’s results are retained:

Laboratory	Sample	Rejected Value	Substituted Value
2	2	0.19	0.06
2	7	0.42	0.20
2	21	0.85	0.61
6	6	0.65	0.85
6	15	1.59, 1.44	0.922

(2) With Laboratory 2’s results omitted, only Laboratory 6’s results listed above were rejected.

X1.4.4 Calculation of Repeatability and Reproducibility:

X1.4.4.1 Repeatability and reproducibility were obtained by fitting curves of the appropriate precision of the results on each sample versus the mean value of each sample. An equation of the form:

$$S = A \bar{x}(1 - e^{-bx}) \quad (\text{X1.1})$$

where:

S = precision,
 \bar{x} = sample mean, and
 A and b = are constants.

was found to best fit the data. The values of the constants A and b were calculated by regression analysis of the linear logarithmic equation:

$$\log S = \log A / \log(1 - e^{-bx}) \quad (\text{X1.2})$$

X1.4.4.2 The standard deviation for repeatability for each sample was calculated from pair-wise (repeat pairs) variances pooled across the laboratories. The standard deviation for reproducibility was calculated from the variance of the mean values of each pair. This variance is equal to the sum of two variances, the variance σ_L^2 due to differences between laboratories and the variance due to repeatability error σ_r^2 divided by the number of replicates:

$$\sigma_r^2 = \sigma_r^2/n + \sigma_L^2(n = 2) \quad (\text{X1.3})$$

Using the data calculated above for each sample, the values listed in Table X1.7 for the constants in Eq X1.1 were obtained. The values of precision calculated by Eq X1.1 were multiplied by $2.828 (2 \times \sqrt{2})$ to convert them to the ASTM-defined repeatability and reproducibility.

X1.4.4.3 The curves of repeatability and reproducibility for the distillation method in the range 0 to 0.09 % water are shown in Fig. X1.1. These data are also tabulated in Table X1.8. The curves for the centrifuge method in the range 0 to 0.2 % water are shown in Fig. X1.2 (five-laboratory case) and Fig. X1.3 (six-laboratory case).

X1.4.4.4 For higher levels of water the limiting repeatabilities and reproducibilities are listed in Table X1.9.

X1.4.4.5 It should be pointed out that at the lowest water levels, the precision “statements” for some of the analyses do not permit any pair of results to be considered suspect. This is because the precision interval exceeds twice the mean value. For example, in Fig. X1.1, the repeatability at 0.03 % water is 0.061 %. It is not possible to observe a difference of more than 0.06 and still average 0.03. Thus, a pair of observations of 0.00 and 0.06 are acceptable.

X1.4.4.6 Analyses of variance were performed on the data without regard to any functionality between water level and precision. The following repeatabilities and reproducibilities were found:

TABLE X1.6 Round-Robin Results of Water in Crude Oils by ASTM D95 (API MPMS Chapter 10.5) and ASTM D1796 (API MPMS Chapter 10.6)

Labora- tories	Distillation Test Method ASTM D95 (API MPMS Chapter 10.5)																				
	Samples																				
	1	9	15	6	18	2	11	19	3	8	13	14	17	20	21	4	5	7	10	12	16
1	0.86	0.90	0.91	0.91	0.88	0.00	0.02	0.00	0.40	0.39	0.46	0.75	0.25	0.35	0.67	0.10	0.15	0.20	0.16	0.13	0.18
	0.86	0.92	0.92	0.86	0.85	0.01	0.02	0.02	0.39	0.40	0.46	0.53	0.38	0.33	0.66	0.09	0.21	0.21	0.20	0.13	0.15
2	0.90	0.94	0.99	0.90	0.90	0.05	0.34	0.04	0.43	0.40	0.48	0.53	0.39	0.35	0.70	0.09	0.25	0.25	0.18	0.11	0.20
	0.91	0.94	1.00	0.92	0.90	0.06	0.06	0.04	0.48	0.40	0.47	0.58	0.36	0.30	0.69	0.11	0.24	0.25	0.19	0.14	0.20
3	0.80	0.94	0.98	0.85	0.90	0.05	0.00	0.00	0.35	0.38	0.45	0.43	0.35	0.33	0.65	0.07	0.20	0.23	0.18	0.05	0.15
	0.85	0.94	0.88	0.83	0.90	0.02	0.03	0.00	0.54	0.40	0.43	0.55	0.33	0.33	0.65	0.10	0.15	0.23	0.15	0.07	0.16
4	0.93	0.92	0.89	0.90	0.88	0.07	0.02	0.00	0.42	0.40	0.42	0.52	0.35	0.35	0.66	0.10	0.19	0.23	0.18	0.10	0.20
	0.93	0.90	0.91	0.89	0.90	0.07	0.02	0.04	0.42	0.39	0.43	0.52	0.33	0.35	0.67	0.10	0.20	0.19	0.16	0.11	0.19
5	0.87	0.88	0.87	0.86	0.86	0.07	0.07	0.05	0.39	0.41	0.42	0.51	0.23	0.39	0.65	0.11	0.21	0.21	0.21	0.16	0.20
	0.86	0.92	0.83	0.80	0.80	0.07	0.09	0.04	0.39	0.40	0.37	0.47	0.35	0.35	0.60	0.12	0.20	0.24	0.24	0.18	0.16
6	0.98	0.94	0.85	0.79	0.74	0.04	0.02	0.00	0.58	0.39	0.45	0.44	0.36	0.38	0.61	0.11	0.24	0.23	0.20	0.07	0.24
	1.01	0.94	1.37	0.84	0.89	0.01	0.00	0.01	0.48	0.80	0.66	0.56	0.30	0.39	0.66	0.13	0.25	0.24	0.21	0.05	0.18
7	0.91	0.88	0.97	0.85	0.80	0.05	0.01	0.01	0.42	0.40	0.41	0.53	0.34	0.36	0.64	0.05	0.18	0.18	0.15	0.18	0.18
	0.97	0.92	1.03	0.84	0.80	0.02	0.13	0.01	0.39	0.35	0.45	0.47	0.35	0.38	0.65	0.15	0.20	0.23	0.15	0.11	0.15
	Centrifuge Test Method D1796 (API MPMS Chapter 10.6)																				
	Samples																				
	1	9	15	6	18	2	11	19	3	8	13	14	17	20	21	4	5	7	10	12	16
1	0.82	0.90	0.87	0.80	0.70	0.05	0.02	0.00	0.23	0.25	0.38	0.48	0.19	0.27	0.65	0.02	0.07	0.05	0.03	0.02	0.02
	0.79	0.89	0.88	0.81	0.74	0.05	0.02	0.02	0.23	0.31	0.35	0.41	0.17	0.29	0.61	0.02	0.06	0.06	0.03	0.02	0.04
2	1.03	1.09	1.06	0.74	0.95	0.19	0.07	0.00	0.19	0.40	0.50	0.58	0.38	0.45	0.61	0.15	0.20	0.20	0.20	0.06	0.20
	0.88	1.11	1.12	0.74	1.00	0.06	0.05	0.00	0.31	0.43	0.58	0.60	0.34	0.50	0.85	0.21	0.37	0.42	0.17	0.06	0.04
3	0.65	0.80	0.90	0.70	0.70	0.07	0.00	0.00	0.10	0.30	0.30	0.42	0.06	0.20	0.60	0.02	0.02	0.07	0.02	0.00	0.02
	0.60	0.85	0.90	0.60	0.70	0.07	0.00	0.02	0.10	0.34	0.40	0.50	0.10	0.20	0.45	0.02	0.02	0.12	0.02	0.00	0.02
4	0.73	0.95	0.88	0.85	0.80	0.00	0.00	0.00	0.18	0.27	0.33	0.46	0.15	0.30	0.63	0.00	0.10	0.10	0.05	0.00	0.05
	0.79	1.00	0.90	0.75	0.70	0.00	0.00	0.00	0.16	0.27	0.40	0.45	0.15	0.27	0.55	0.00	0.05	0.13	0.05	0.00	0.05
5	0.69	1.55	0.51	0.87	0.83	0.01	0.03	0.03	0.18	0.21	0.16	0.30	0.21	0.39	0.72	0.75	0.13	0.01	0.21	0.03	0.05
	0.76	1.10	0.87	0.93	0.41	0.01	0.05	0.02	0.30	0.54	0.20	0.07	0.19	0.01	0.69	0.06	0.11	0.02	0.09	0.03	0.12
6	0.72	0.75	1.59	0.85	0.65	0.07	0.05	0.05	0.35	0.33	0.25	0.52	0.20	0.45	0.75	0.05	0.15	0.05	0.05	0.05	0.05
	0.86	0.90	1.44	0.65	0.65	0.09	0.05	0.05	0.32	0.25	0.38	0.52	0.25	0.38	0.80	0.10	0.10	0.13	0.10	0.05	0.10
7	0.88	1.00	0.85	0.85	0.70	0.00	0.00	0.05	0.15	0.20	0.30	0.40	0.25	0.23	0.63	0.10	0.18	0.25	0.20	0.00	0.18
	0.90	0.85	0.80	0.80	0.80	0.00	0.00	0.05	0.10	0.35	0.30	0.35	0.13	0.25	0.60	0.18	0.20	0.30	0.15	0.00	0.10

TABLE X1.7 Constants (see Eq X1.1)

Constant	Distillation Method 7 Laboratories		Centrifuge Method 6 Laboratories		Centrifuge Method 5 Laboratories	
	Repeatability	Reproducibility	Repeatability	Reproducibility	Repeatability	Reproducibility
<i>b</i>	47.41	47.41	11.23	11.23	17.87	17.87
<i>A</i>	0.2883	0.0380	0.0441	0.1043	0.0437	0.0658

Method	Repeatability	Reproducibility
Distillation (seven laboratories)	0.08	0.11
Centrifuge (six laboratories)	0.12	0.28

These values are almost exactly the same as the limiting values obtained by curve fitting.

X1.5 Conclusions and Recommendations

X1.5.1 Data obtained in seven-laboratory round robin on measurement of basic sediment and water by the distillation test method, Test Method D95 (API MPMS Chapter 10.5) and

the centrifuge test method, Test Method D1796 (API MPMS Chapter 10.6) in 21 crude oil samples were examined. The conclusions are:

X1.5.1.1 Distillation Method:

(1) Precision is related to water content up to about 0.10 % water.

(2) In the range from 0.01 to 0.10, repeatability varies from 0.020 to 0.078 and reproducibility from 0.041 to 0.105.

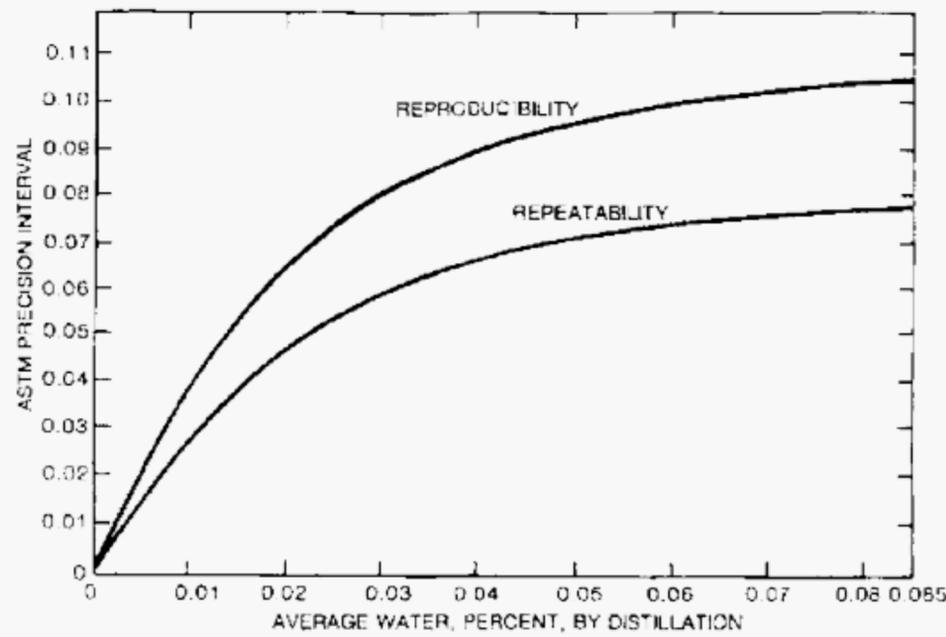


FIG. X1.1 Basic Sediment and Water Precision for ASTM Test Method D95 (API MPMS Chapter 10.5) Distillation (Based on Seven Laboratories)

TABLE X1.8 ASTM Precision Intervals: ASTM D95 (API MPMS Chapter 10.5) (7 Laboratories)

% Water	Repeatability	Reproducibility	% Water
0.000	0.000	0.000	0.000
0.005	0.017	0.023	0.005
0.010	0.030	0.041	0.010
0.015	0.041	0.055	0.015
0.020	0.049	0.066	0.020
0.025	0.056	0.075	0.025
0.030	0.061	0.082	0.030
0.035	0.065	0.087	0.035
0.040	0.068	0.091	0.040
0.045	0.071	0.095	0.045
0.050	0.073	0.097	0.050
0.055	0.074	0.100	0.055
0.060	0.075	0.101	0.060
0.065	0.076	0.103	0.065
0.070	0.077	0.104	0.070
0.075	0.078	0.104	0.075
0.080	0.078	0.105	0.080
0.085	0.079	0.106	0.085
0.090	0.079	0.106	0.090
0.095	0.079	0.106	0.095
0.100	0.079	0.107	0.100
0.105	0.079	0.107	0.105
0.110	0.080	0.107	0.110
0.115	0.080	0.107	0.115
0.120	0.080	0.107	0.120
0.125	0.080	0.107	0.125
0.130	0.080	0.107	0.130

(3) Above 0.1 % water, the repeatability is 0.08 and the reproducibility is 0.11.

X1.5.1.2 Centrifuge Method:

(1) Repeatability is related to water content up to about 0.2 % water and reproducibility up to about 0.3 %.

(2) In the range 0.01 to 0.2, repeatability varies from 0.01 to 0.11 and reproducibility in the range 0.02 to 0.3 from 0.03 to 0.28.

X1.5.2 It is recommended that:

X1.5.2.1 Precision should be presented as a graph in the range where precision varies with water content.

X1.5.2.2 Precision should be presented as a statement where the precision is constant.

X1.5.3 In view of what appears to be lower bias and better precision, Test Method D95 (API MPMS Chapter 10.5) should be the specified method for use in critical situations.

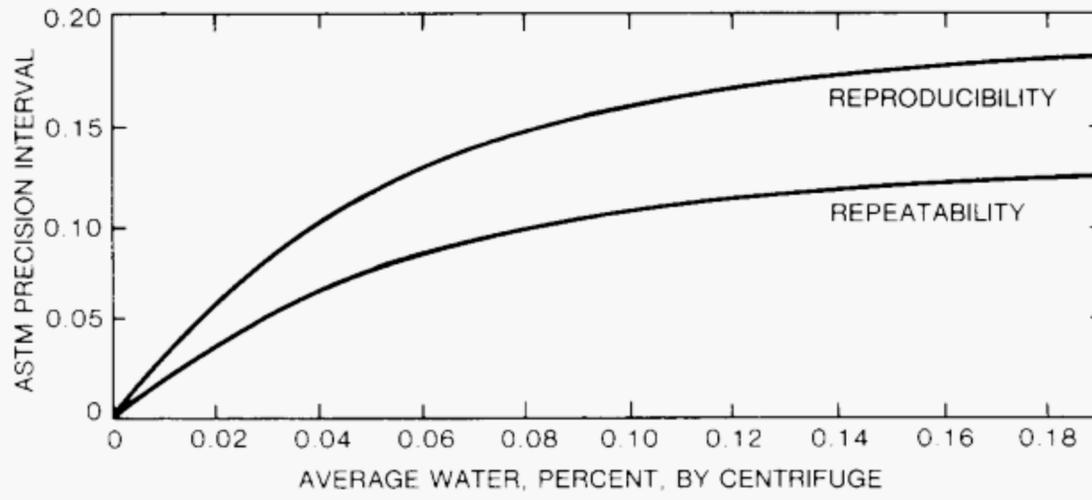


FIG. X1.2 Basic Sediment and Water Precision for ASTM Test Method D1796 (API MPMS Chapter 10.6) Centrifuge (Based on Five Laboratories)

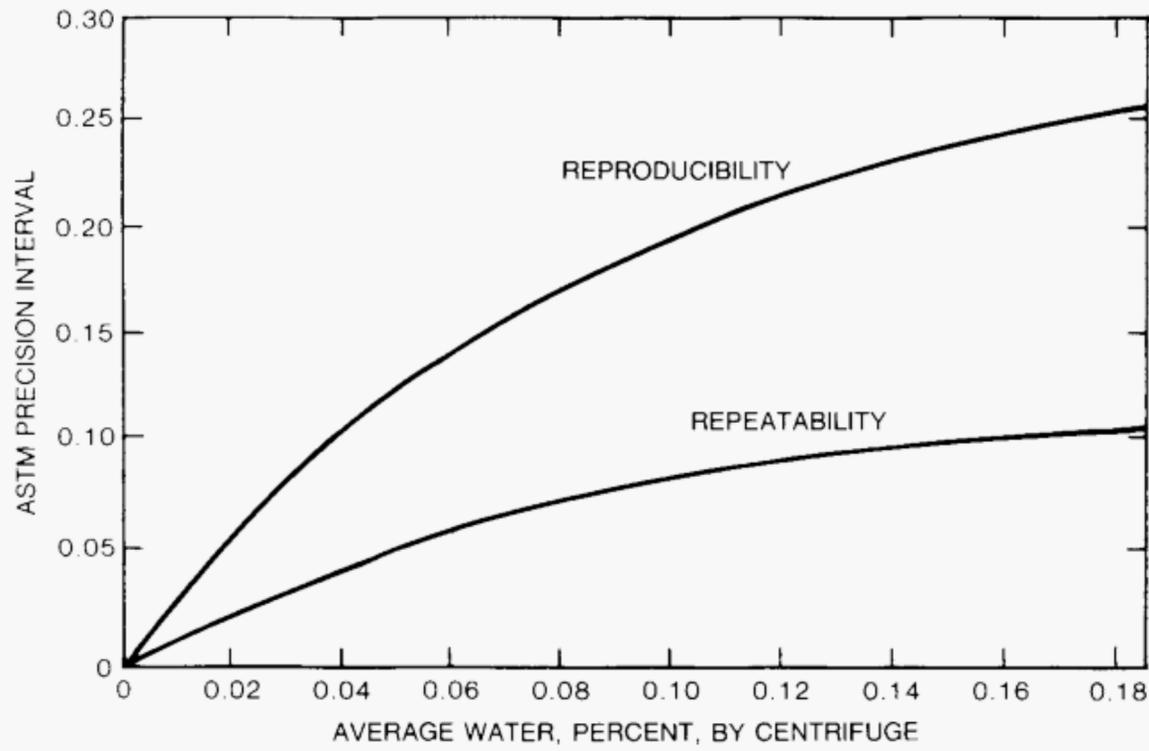


FIG. X1.3 Basic Sediment and Water Precision for ASTM Test Method D1796 (API MPMS Chapter 10.6) Centrifuge (Based on Six Laboratories)

TABLE X1.9 Limiting Repeatabilities and Reproducibilities

Method	Repeatability		Reproducibility	
	Range of Concentration, %	Value, %	Range of Concentration, %	Value, %
Distillation	≥ 0.085	0.08	≥ 0.085	0.105
Centrifuge (five-laboratory case)	≥ 0.155	0.12	≥ 0.325	0.19
Centrifuge (six-laboratory case)	≥ 0.235	0.12	≥ 0.315	0.29

SUMMARY OF CHANGES

Subcommittee D02.02.07 has identified the location of selected changes to this standard since the last issue (D4007–08) that may impact the use of this standard.

- (1) Added Test Method **D4928** to Referenced Documents and standard text. (2) Added Subsection **4.2**.

EXPLORE SOME MORE

Check out more of API's certification and training programs, standards, statistics and publications.

API Monogram™ Licensing Program

Sales: 877-562-5187
(Toll-free U.S. and Canada)
(+1) 202-682-8041
(Local and International)
Email: certification@api.org
Web: www.api.org/monogram

API Quality Registrar (APIQR™)

- ISO 9001
- ISO/TS 29001
- ISO 14001
- OHSAS 18001
- API Spec Q1®
- API Spec Q2™
- API Quality Plus™
- Dual Registration

Sales: 877-562-5187
(Toll-free U.S. and Canada)
(+1) 202-682-8041
(Local and International)
Email: certification@api.org
Web: www.api.org/apiqr

API Training Provider Certification Program (API TPCP®)

Sales: 877-562-5187
(Toll-free U.S. and Canada)
(+1) 202-682-8041
(Local and International)
Email: tpcp@api.org
Web: www.api.org/tpcp

API Individual Certification Programs (ICP™)

Sales: 877-562-5187
(Toll-free U.S. and Canada)
(+1) 202-682-8041
(Local and International)
Email: icp@api.org
Web: www.api.org/icp

API Engine Oil Licensing and Certification System (EOLCS™)

Sales: 877-562-5187
(Toll-free U.S. and Canada)
(+1) 202-682-8041
(Local and International)
Email: eolcs@api.org
Web: www.api.org/eolcs

Motor Oil Matters™

Sales: 877-562-5187
(Toll-free U.S. and Canada)
(+1) 202-682-8041
(Local and International)
Email: motoroilmatters@api.org
Web: www.motoroilmatters.org

API Diesel Exhaust Fluid™ Certification Program

Sales: 877-562-5187
(Toll-free U.S. and Canada)
(+1) 202-682-8041
(Local and International)
Email: apidef@api.org
Web: www.apidef.org

API Perforator Design™ Registration Program

Sales: 877-562-5187
(Toll-free U.S. and Canada)
(+1) 202-682-8041
(Local and International)
Email: perfdesign@api.org
Web: www.api.org/perforators

API WorkSafe™

Sales: 877-562-5187
(Toll-free U.S. and Canada)
(+1) 202-682-8041
(Local and International)
Email: apiworksafe@api.org
Web: www.api.org/worksafe

API-U®

Sales: 877-562-5187
(Toll-free U.S. and Canada)
(+1) 202-682-8041
(Local and International)
Email: training@api.org
Web: www.api-u.org

API eMaintenance™

Sales: 877-562-5187
(Toll-free U.S. and Canada)
(+1) 202-682-8041
(Local and International)
Email: apiemaint@api.org
Web: www.apiemaintenance.com

API Standards

Sales: 877-562-5187
(Toll-free U.S. and Canada)
(+1) 202-682-8041
(Local and International)
Email: standards@api.org
Web: www.api.org/standards

API Data™

Sales: 877-562-5187
(Toll-free U.S. and Canada)
(+1) 202-682-8041
(Local and International)
Service: (+1) 202-682-8042
Email: data@api.org
Web: www.api.org/data

API Publications

Phone: 1-800-854-7179
(Toll-free U.S. and Canada)
(+1) 303-397-7956
(Local and International)
Fax: (+1) 303-397-2740
Web: www.api.org/pubs
global.ihs.com



AMERICAN PETROLEUM INSTITUTE

1220 L Street, NW
Washington, DC 20005-4070
USA

202-682-8000

Additional copies are available online at www.api.org/pubs

Phone Orders: 1-800-854-7179 (Toll-free in the U.S. and Canada)
303-397-7956 (Local and International)

Fax Orders: 303-397-2740

Information about API publications, programs and services is available
on the web at www.api.org.

Product No. H100304