

AS ISO 19976.1:2020  
ISO 19976-1:2019



STANDARDS  
Australia



# Copper, lead and zinc sulfide concentrates — Determination of cadmium

## Part 1: Flame atomic absorption spectrometric method



AS ISO 19976.1:2020

This Australian Standard® was prepared by MN-005, Copper, Lead, Zinc and Nickel Ores and Concentrates. It was approved on behalf of the Council of Standards Australia on 2 September 2020.

This Standard was published on 11 September 2020.

The following are represented on Committee MN-005:

- Australasian Institute of Mining & Metallurgy
- Australian X-ray Analytical Association
- Chamber of Minerals and Energy of Western Australia
- CSIRO
- International Copper Association Australia
- Minerals Council of Australia
- Queensland Resources Council

This Standard was issued in draft form for comment as DR AS ISO 19976.1:2020.

### **Keeping Standards up-to-date**

Ensure you have the latest versions of our publications and keep up-to-date about Amendments, Rulings, Withdrawals, and new projects by visiting:

[www.standards.org.au](http://www.standards.org.au)

ISBN 978 1 76072 977 6

# **Copper, lead and zinc sulfide concentrates — Determination of cadmium**

## **Part 1: Flame atomic absorption spectrometric method**

First published as AS ISO 19976.1:2020.

### **COPYRIGHT**

© ISO 2020 — All rights reserved  
© Standards Australia Limited 2020

All rights are reserved. No part of this work may be reproduced or copied in any form or by any means, electronic or mechanical, including photocopying, without the written permission of the publisher, unless otherwise permitted under the Copyright Act 1968 (Cth).



## Preface

This Standard was prepared by the Standards Australia Committee MN-005, Copper, Lead, Zinc and Nickel Ores and Concentrates.

The objective of this document is to specify a flame atomic absorption spectrometric method for the determination of the mass fraction of cadmium in copper, lead and zinc sulfide concentrates as follows:

- (a) For copper sulfide concentrates, the method is applicable to the determination of mass fractions of cadmium from 0.01 % to 0.30 %.
- (b) For lead sulfide concentrates, the method is applicable to the determination of mass fractions of cadmium from 0.01 % to 0.30 %.
- (c) For zinc sulfide concentrates, the method is applicable to the determination of mass fractions of cadmium from 0.05 % to 0.30 %.

This document is identical with, and has been reproduced from, ISO 19976-1:2019, *Copper, lead and zinc sulfide concentrates — Determination of cadmium — Part 1: Flame atomic absorption spectrometric method*.

As this document has been reproduced from an International Standard, a full point substitutes for a comma when referring to a decimal marker.

Australian or Australian/New Zealand Standards that are identical adoptions of international normative references may be used interchangeably. Refer to the online catalogue for information on specific Standards.

The terms “normative” and “informative” are used in Standards to define the application of the appendices or annexes to which they apply. A “normative” appendix or annex is an integral part of a Standard, whereas an “informative” appendix or annex is only for information and guidance.

# Contents

<b>Preface</b> .....	<b>ii</b>
<b>Foreword</b> .....	<b>iv</b>
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative reference</b> .....	<b>1</b>
<b>3 Terms and definitions</b> .....	<b>1</b>
<b>4 Principle</b> .....	<b>2</b>
<b>5 Reagents</b> .....	<b>2</b>
<b>6 Apparatus</b> .....	<b>3</b>
<b>7 Samples</b> .....	<b>3</b>
7.1 Laboratory sample .....	3
7.2 Test sample .....	3
7.3 Test portion .....	3
<b>8 Procedure</b> .....	<b>4</b>
8.1 Number of determinations .....	4
8.2 Blank test .....	4
8.3 Determination .....	4
8.3.1 Dissolution of test portion .....	4
8.3.2 Preparation of test solutions .....	4
8.3.3 Adjustment of the AAS .....	5
8.3.4 Atomic absorption measurements .....	5
8.4 Check test .....	5
<b>9 Expression of results</b> .....	<b>5</b>
<b>10 Precision and accuracy</b> .....	<b>6</b>
10.1 Expression of precision .....	6
10.2 Method for obtaining the final result .....	6
10.3 Between-laboratories precision .....	6
10.4 Check of trueness .....	7
10.4.1 General .....	7
10.4.2 Type of CRM or reference material .....	7
<b>11 Test report</b> .....	<b>8</b>
<b>Annex A</b> (informative) <b>Procedure for the preparation and determination of the mass of a predried test portion</b> .....	<b>9</b>
<b>Annex B</b> (normative) <b>Procedure for obtaining the final result</b> .....	<b>11</b>
<b>Bibliography</b> .....	<b>12</b>



## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).

This document was prepared by Technical Committee ISO/TC 183, *Copper, lead, zinc and nickel ores and concentrates*.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at [www.iso.org/members.html](http://www.iso.org/members.html).



# Australian Standard®

## Copper, lead and zinc sulfide concentrates — Determination of cadmium Part 1: Flame atomic absorption spectrometric method

**WARNING — The use of this document might involve hazardous materials, operations and equipment. It is the responsibility of the user of this document to establish appropriate health and safety practices.**

### 1 Scope

This document specifies a flame atomic absorption spectrometric method for the determination of the mass fraction of cadmium in copper, lead and zinc sulfide concentrates as follows:

- a) for copper sulfide concentrates, the method is applicable to the determination of mass fractions of cadmium from 0,01 % to 0,30 %;
- b) for lead sulfide concentrates, the method is applicable to the determination of mass fractions of cadmium from 0,01 % to 0,30 %;
- c) for zinc sulfide concentrates, the method is applicable to the determination of mass fractions of cadmium from 0,05 % to 0,30 %.

### 2 Normative reference

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 385, *Laboratory glassware — Burettes*

ISO 648, *Laboratory glassware — Single-volume pipettes*

ISO 1042, *Laboratory glassware — One-mark volumetric flasks*

ISO 4787, *Laboratory glassware — Volumetric instruments — Methods for testing of capacity and for use*

ISO 9599, *Copper, lead, zinc and nickel sulfide concentrates — Determination of hygroscopic moisture content of the analysis sample — Gravimetric method*

ISO 12743, *Copper, lead, zinc and nickel concentrates — Sampling procedures for determination of metal and moisture content*

ISO Guide 35, *Reference materials — Guidance for characterization and assessment of homogeneity and stability*

### 3 Terms and definitions

No terms and definitions are listed in this document.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>



## 4 Principle

Dissolve the test portion in hydrochloric acid and nitric acid. Add hydrofluoric acid to remove silicon. Then add perchloric acid and determine the iron concentration in the test portion using an atomic absorption spectrometer (AAS) with a deuterium lamp for background correction at 228,8 nm.

## 5 Reagents

During the analysis, use only reagents of recognized analytical grade and distilled water or water of equivalent purity.

**5.1 Hydrochloric acid**, concentrated ( $\rho_{20}$  1,19 g/ml).

**5.2 Hydrochloric acid**, diluted 1+1.

Slowly add 500 ml of concentrated hydrochloric acid (5.1) to 500 ml of water, while stirring.

**5.3 Hydrochloric acid**, diluted 1+9.

Slowly add 50 ml of concentrated hydrochloric acid (5.1) to 450 ml of water, while stirring.

**5.4 Nitric acid**, concentrated ( $\rho_{20}$  1,42 g/ml).

**5.5 Hydrofluoric acid**, concentrated ( $\rho_{20}$  1,15 g/ml).

**5.6 Perchloric acid**, concentrated ( $\rho_{20}$  1,70 g/ml).

**5.7 Cadmium metal**, minimum purity 99,99 %.

**5.8 Cadmium**, standard solution, 1 ml contains 1 mg of Cd.

Weigh, to the nearest 0,1 mg, 1,000 0 g of cadmium metal (5.7) into a 250 ml beaker. Add 10 ml of water and 5 ml of nitric acid (5.4). Cover and warm gently (if necessary) until the cadmium metal is dissolved. Heat to remove nitrogen oxides, then allow to cool and add about 50 ml of water. Transfer the solution to a 1 000 ml one-mark volumetric flask, add 40 ml of hydrochloric acid (5.2), fill up nearly to the mark with water, mix and cool to room temperature, then fill up exactly to the mark with water and mix again.

**5.9 Cadmium**, standard solution, 1 ml contains 100 µg of Cd.

Pipette 10,00 ml of cadmium standard solution (5.8) into a 100 ml one-mark volumetric flask. Add 20 ml of hydrochloric acid (5.2), fill up nearly to the mark with water, mix and cool to room temperature, then fill up exactly to the mark with water and mix again.

**5.10 Cadmium**, standard solution, 1 ml contains 10 µg of Cd.

Pipette 10,00 ml of cadmium standard solution (5.9) into a 100 ml one-mark volumetric flask. Add 18 ml of hydrochloric acid (5.2), fill up nearly to the mark with water, mix and cool to room temperature, then fill up exactly to the mark with water and mix again.

**5.11 Cadmium calibration solutions.**

Prepare a series of calibration solutions by adding, from a pipette, 0,0 ml, 2,00 ml, 4,00 ml, 6,00 ml, 7,00 ml, 8,00 ml, 9,00 ml and 10,00 ml of cadmium standard solution (5.10) into a series of 100 ml one-mark volumetric flasks. Dilute to the mark with hydrochloric acid (5.3) and mix thoroughly.



These standards contain 0,0 µg, 0,2 µg, 0,4 µg, 0,6 µg, 0,7 µg, 0,8 µg, 0,9 µg and 1,0 µg of cadmium per ml and shall be freshly prepared.

Calibration solutions should be prepared at the same ambient temperature as that at which the determinations will be conducted.

## 6 Apparatus

Ordinary laboratory equipment and the following.

**6.1 Volumetric glassware**, of class A conforming with ISO 385, ISO 648 and ISO 1042, and used in accordance with ISO 4787.

It is permissible to use other measuring instruments, approved types, auxiliary devices and materials whose technical and metrological characteristics are not inferior to those mentioned above.

**6.2 Polytetrafluoroethylene beaker**, of capacity 200 ml, or glass-carbon beaker.

**6.3 Analytical balance**, sensitive to 0,1 mg.

**6.4 AAS**, equipped with a cadmium hollow cathode lamp and deuterium lamp for background correction.

Recommended instrument conditions:

- flame: air-acetylene;
- wavelength: 228,8 nm;
- slit width: 0,2 nm.

**6.5 Insolubles filter paper**, Whatman®<sup>1)</sup> No. 40 or equivalent.

## 7 Samples

### 7.1 Laboratory sample

Laboratory samples shall be taken and prepared in accordance with the procedures described in ISO 12743.

### 7.2 Test sample

Prepare an air-equilibrated test sample in accordance with ISO 9599.

NOTE A test sample is not required if pre-dried test portions are to be used (see [Annex A](#)).

### 7.3 Test portion

Taking multiple increments, extract approximately 0,50 g from the test sample and weigh to the nearest 0,1 mg. At the same time as test portions are being weighed for analysis, weigh test portions for the determination of hygroscopic moisture in accordance with ISO 9599.

Alternatively, the method specified in [Annex A](#) can be used to prepare pre-dried test portions directly from the laboratory sample.

---

1) This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of the product named. Equivalent products may be used if they can be shown to lead to the same results.



## 8 Procedure

### 8.1 Number of determinations

Carry out the determinations at least in duplicate, as far as possible under repeatability conditions, on each test sample.

NOTE Repeatability conditions exist where mutually independent test results are obtained with the same method on identical test material in the same laboratory by the same operator using the same equipment, within short intervals of time.

### 8.2 Blank test

Carry out a blank test in parallel with the analysis using the same quantities of all reagents but omitting the test portion. The purpose of the blank test in this method is to check the quality of reagents. If a significant blank value is obtained as a result of the blank test, check all reagents and rectify the problem.

### 8.3 Determination

#### 8.3.1 Dissolution of test portion

Transfer the test portion into a 200 ml polytetrafluoroethylene beaker (6.2) and moisten with 5 ml of water.

Add 10 ml of hydrochloric acid (5.1) and heat for 5 min at 60 °C to 70 °C. Add 10 ml of nitric acid (5.4) and heat gently. Add 3 ml of hydrofluoric acid (5.5), then heat gradually until the solution is about 5 ml at 60 °C to 70 °C. Add perchloric acid (5.6) repeatedly until the residue is not present. Heat until the strong white fumes have exhausted completely, then allow to cool.

Add 40 ml of hydrochloric acid (5.2) [for lead concentrate samples, add 50 ml of hydrochloric acid (5.3)]. Wash down the cover and sides of the beaker and then heat until the onset of boiling, then allow to cool.

#### 8.3.2 Preparation of test solutions

Transfer the solution (8.3.1) to a 200 ml one-mark volumetric flask, dilute to the mark with water and mix thoroughly [for lead concentrate samples, filter the solution through an insoluble filter paper (6.5)]. Wash the precipitate with hydrochloric acid (5.3) and collect the filtrate in a 200 ml one-mark volumetric flask. Dilute to the mark with hydrochloric acid (5.3) and mix thoroughly. Then transfer an appropriate aliquot of this solution (see Table 1) to the corresponding one-mark volumetric flask. Add an appropriate amount of hydrochloric acid (5.2) as indicated in Table 1, fill up nearly to the mark with water, mix and cool to room temperature, then fill up exactly to the mark with water and mix again.

The dilutions shown in Table 1 will provide concentrations of cadmium falling within the range of the calibration solutions.

**Table 1 — Dilution guide for test solution**

Expected mass fraction of cadmium in sample $w_{Cd}/\%$	Aliquot to take $V_1/\text{ml}$	Hydrochloric acid (5.2) to be added ml	Volume after dilution $V_2/\text{ml}$
$0,01 \leq w_{Cd} \leq 0,03$	—	—	—
$0,03 < w_{Cd} \leq 0,08$	20,00	6,0	50
$0,08 < w_{Cd} \leq 0,30$	10,00	18,0	100



### 8.3.3 Adjustment of the AAS

Fit the cadmium hollow-cathode lamp into the apparatus (6.4), switch on the current and allow to stabilize. Adjust the current, the sensitivity and the aperture of the slit according to the characteristics of the apparatus. Adjust the wavelength in the region of 228,8 nm to obtain maximum absorbance. Adjust the pressure of air and acetylene according to the characteristics of the aspirator burner.

### 8.3.4 Atomic absorption measurements

Aspirate the calibration solutions (5.11) and the final test solution (see 8.3.2) into the AAS (6.4) and measure the absorbance. As a guide, the instrument should be as near as is practical to a linear relationship between absorbance and concentration.

Perform three measurements on each standard solution. Calculate, to three significant figures, the mean absorbance for each standard solution, provided that the range of values does not exceed 0,003 absorbance units. If this range is exceeded, repeat the calibration.

The test solutions should be treated in the same manner. Plot a calibration graph of absorbance versus concentration of cadmium.

## 8.4 Check test

Make a preliminary check of the apparatus by preparing a solution of standard material or a synthetic sample containing a known amount of cadmium and of composition similar to the material to be analysed, and carry out the procedure as specified in 8.3.

## 9 Expression of results

The mass fraction of cadmium in the test portion,  $w_{Cd}$ , expressed as a percentage, is given by Formula (1).

$$w_{Cd} = \frac{(\rho - \rho_0) \cdot V \cdot V_2}{m \cdot V_1 \times 10^6} \times \frac{100}{100 - H} \times 100 \quad (1)$$

where

- $\rho$  is the concentration, in micrograms per millilitre, of cadmium in the test solution obtained from the calibration curve;
- $\rho_0$  is the concentration, in micrograms per millilitre, of cadmium in the blank solution;
- $V$  is the total volume, in millilitres, of test solution before transferring the aliquot solution;
- $V_1$  is the volume, in millilitres, of aliquot solution to be transferred;
- $V_2$  is the volume, in millilitres, of test solution after dilution;
- $m$  is the mass, in grams, of the test portion;
- $H$  is the hygroscopic moisture content of the sample, expressed as a percentage, determined using ISO 9599.

NOTE If pre-dried test samples are used,  $H = 0$ .

Calculate the mass fraction of cadmium in the test portion to the second decimal place, and to the third decimal place if the mass fraction of cadmium is less than 0,1 %.

## 10 Precision and accuracy

### 10.1 Expression of precision

The precision of this analytical method is expressed by [Formulae \(2\) to \(7\)](#).

a) for copper concentrates:

$$s_r = 0,0114 \bar{X} \quad (2)$$

$$s_L = 0,0150 \bar{X} + 0,0004 \quad (3)$$

b) for lead concentrates:

$$s_r = 0,0262 \bar{X} \quad (4)$$

$$s_L = 0,0382 \bar{X} - 0,0002 \quad (5)$$

c) for zinc concentrates:

$$s_r = 0,0101 \bar{X} + 0,0004 \quad (6)$$

$$s_L = 0,0283 \bar{X} - 0,0005 \quad (7)$$

where

$\bar{X}$  is the mean mass fraction of cadmium in the sample, expressed as a percentage;

$s_r$  is the within-laboratory standard deviation, expressed as a percentage by mass of cadmium;

$s_L$  is the between-laboratories standard deviation, expressed as a percentage by mass of cadmium.

### 10.2 Method for obtaining the final result

Calculate the quantities in [Formula \(8\)](#) and [Formula \(9\)](#) from the duplicate results  $x_1$  and  $x_2$  (%) and process according to the flowchart in [Annex B](#).

a) Mean of duplicates:

$$\bar{x} = \frac{x_1 + x_2}{2} \quad (8)$$

Within-laboratory standard deviation ( $s_r$ ), using [Formula \(2\)](#) for copper sulfide concentrates, [Formula \(4\)](#) for lead sulfide concentrates and [Formula \(6\)](#) for zinc sulfide concentrates.

b) Repeatability limit:

$$r = 2,8s_r \quad (9)$$

### 10.3 Between-laboratories precision

The between-laboratories precision is used to determine the agreement between the results reported by two (or more) laboratories. The assumption is that all laboratories followed the same procedure.



Calculate the quantities in [Formula \(10\)](#) to [Formula \(12\)](#).

a) Mean of final results:

$$m_{12} = \frac{m_1 + m_2}{2} \quad (10)$$

Between-laboratories standard deviation ( $s_L$ ) substitutes  $\mu_{12}$  for  $\bar{X}$  when using [Formula \(3\)](#) for copper sulfide concentrates, [Formula \(5\)](#) for lead sulfide concentrates and [Formula \(7\)](#) for zinc sulfide concentrates.

Within-laboratory standard deviation ( $s_r$ ) substitutes  $\mu_{12}$  for  $\bar{X}$  when using [Formula \(2\)](#) for copper sulfide concentrates, [Formula \(4\)](#) for lead sulfide concentrates and [Formula \(6\)](#) for zinc sulfide concentrates.

b) Permissible difference

$$P = 2,8 \cdot \sqrt{s_L^2 + \frac{s_r^2}{2}} \quad (11)$$

c) Range:

$$E = |m_1 - m_2| \quad (12)$$

where

$\mu_1$  is the final result reported by laboratory 1, expressed as a percentage by mass of cadmium;

$\mu_2$  is the final result reported by laboratory 2, expressed as a percentage by mass of cadmium.

If  $E \leq P$ , the final results are in agreement.

## 10.4 Check of trueness

### 10.4.1 General

The trueness of the analytical method can be checked by applying it to a certified reference material (CRM). When the precision has been confirmed, the final laboratory result can be compared with the certified value,  $A_c$ . The two possibilities shown in [Formula \(13\)](#) and [Formula \(14\)](#) exist.

$$|m_{\text{c}} - A_{\text{c}}| \leq C \quad (13)$$

where

$\mu_c$  is the final result, expressed as a percentage by mass of cadmium of the CRM;

$A_c$  is the certified value, expressed as a percentage by mass of cadmium of the CRM;

$C$  is a quantity, expressed as a percentage by mass of cadmium depending on the type of the CRM used as defined in [10.4.2](#).

#### 10.4.2.2 Reference material certified/characterized by inter-laboratory test programme

The quantity  $C$  (see 10.4.1), expressed as a percentage by mass of cadmium, is given by Formula (15).

$$C = 2 \times \sqrt{s_L^2 + \frac{s_r^2}{n} + s^2(A_c)} \quad (15)$$

where

$s^2(A_c)$  is the variance of the certified value;

$n$  is the number of replicate determinations.

#### 10.4.2.3 Reference material certified/characterized by one laboratory

The quantity  $C$  (see 10.4.1), expressed as a percentage by mass of cadmium, is given by Formula (16).

$$C = \sqrt{s_L^2 + \frac{s_r^2}{n}} \quad (16)$$

It is recommended that this type of CRM should be avoided, unless the particular CRM is known to have an unbiased certified value.

## 11 Test report

The test report shall contain the following information:

- a) a reference to this document;
- b) identification of the sample;
- c) the mass fraction of cadmium in the sample, expressed as a percentage;
- d) the date on which the test was carried out;
- e) any occurrences noticed during the determination which may have had an influence on the results.



## **Annex A**

### **(informative)**

# **Procedure for the preparation and determination of the mass of a predried test portion**

## **A.1 Scope**

This annex specifies a method for the preparation and determination of the mass of a predried test portion in the analysis of copper, lead and zinc sulfide concentrates.

The method is applicable to copper, lead and zinc sulfide concentrates not susceptible to oxidation and with hygroscopic moisture contents ranging from 0,05 % to 2 %.

## **A.2 Principle**

The test portion to be used for analysis is dried in air in an oven maintained at  $105\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$ . The dried test portion is then weighed and used for the analysis. No correction for hygroscopic moisture is required.

## **A.3 Chemicals**

**A.3.1 Desiccant**, such as self-indicating silica gel or anhydrous magnesium perchlorate.

**WARNING** — Care must be taken when disposing of exhausted magnesium perchlorate. It must be washed down the sink with a stream of running water.

## **A.4 Apparatus**

Ordinary laboratory equipment, and the following.

**A.4.1 Analytical balance**, sensitive to 0,1 mg.

**A.4.2 Weighing vessels**, of glass or silica or corrosion-resistant metal, with externally fitting airtight covers. For small test portions (of mass less than 3 g), the mass of the vessel shall be as small as possible, i.e. less than 20 g.

**A.4.3 Laboratory oven**, capable of maintaining a temperature of  $105\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$ .

## **A.5 Procedure**

### **A.5.1 Preparation of the weighing vessel**

Dry the weighing vessel and its cover ([A.4.2](#)) by heating in the laboratory oven ([A.4.3](#)) at  $105\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$  for 1 h. Transfer the vessel and its cover to a desiccator containing a suitable fresh desiccant ([A.3.1](#)) and allow to cool to ambient temperature.

### A.5.2 Test portion

Tare the dried weighing vessel and its cover (A.5.1). Immediately add the mass of laboratory sample specified for analysis. An accurate total mass of the test portion and weighing vessel is not required at this point.

### A.5.3 Determination of the test portion dry mass

Transfer the uncovered weighing vessel and the test portion and the vessel cover to the laboratory oven (A.4.3) and dry at  $105\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$  for 2 h. After the 2 h period, remove the weighing vessel and dry test portion from the oven, replace the vessel cover and allow to cool to ambient temperature in the desiccator. When cool, remove the weighing vessel containing the dry test portion and the vessel cover from the desiccator, and weigh to the nearest 0,1 mg ( $m_1$ ) after slightly lifting the cover and quickly replacing it.

Transfer the test portion into the appropriate analytical apparatus and immediately reweigh the empty weighing vessel and its cover. Record the mass ( $m_2$ ) to the nearest 0,1 mg.

For new concentrates of unknown characteristics, it is advisable to repeat the drying for another 2 h at  $105\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$ , and to reweigh the weighing vessel containing the test portion and the vessel cover to the nearest 0,1 mg ( $m_1'$ ). The mass of the test portion can be considered to be constant if the difference ( $m_1 - m_1'$ ) is less than or equal to 0,5 mg. If this condition is not achieved, the drying and weighing steps should be repeated.

## A.6 Calculation of the dry mass of the test portion

The dry mass of the test portion ( $m_3$ , in grams) is given by Formula (A.1).

$$m_3 = m_1 - m_2 \quad (\text{A.1})$$

where

$m_1$  is the mass, in grams, of the dried test portion plus the weighing vessel and its cover;


$m_2$  is the mass, in grams, of the empty weighing vessel plus its cover.

The mass of the dry test portion is the mass to be used to calculate the element content in the laboratory sample on a dry basis. No correction for hygroscopic moisture is required.



## Annex B (normative)

### Procedure for obtaining the final result

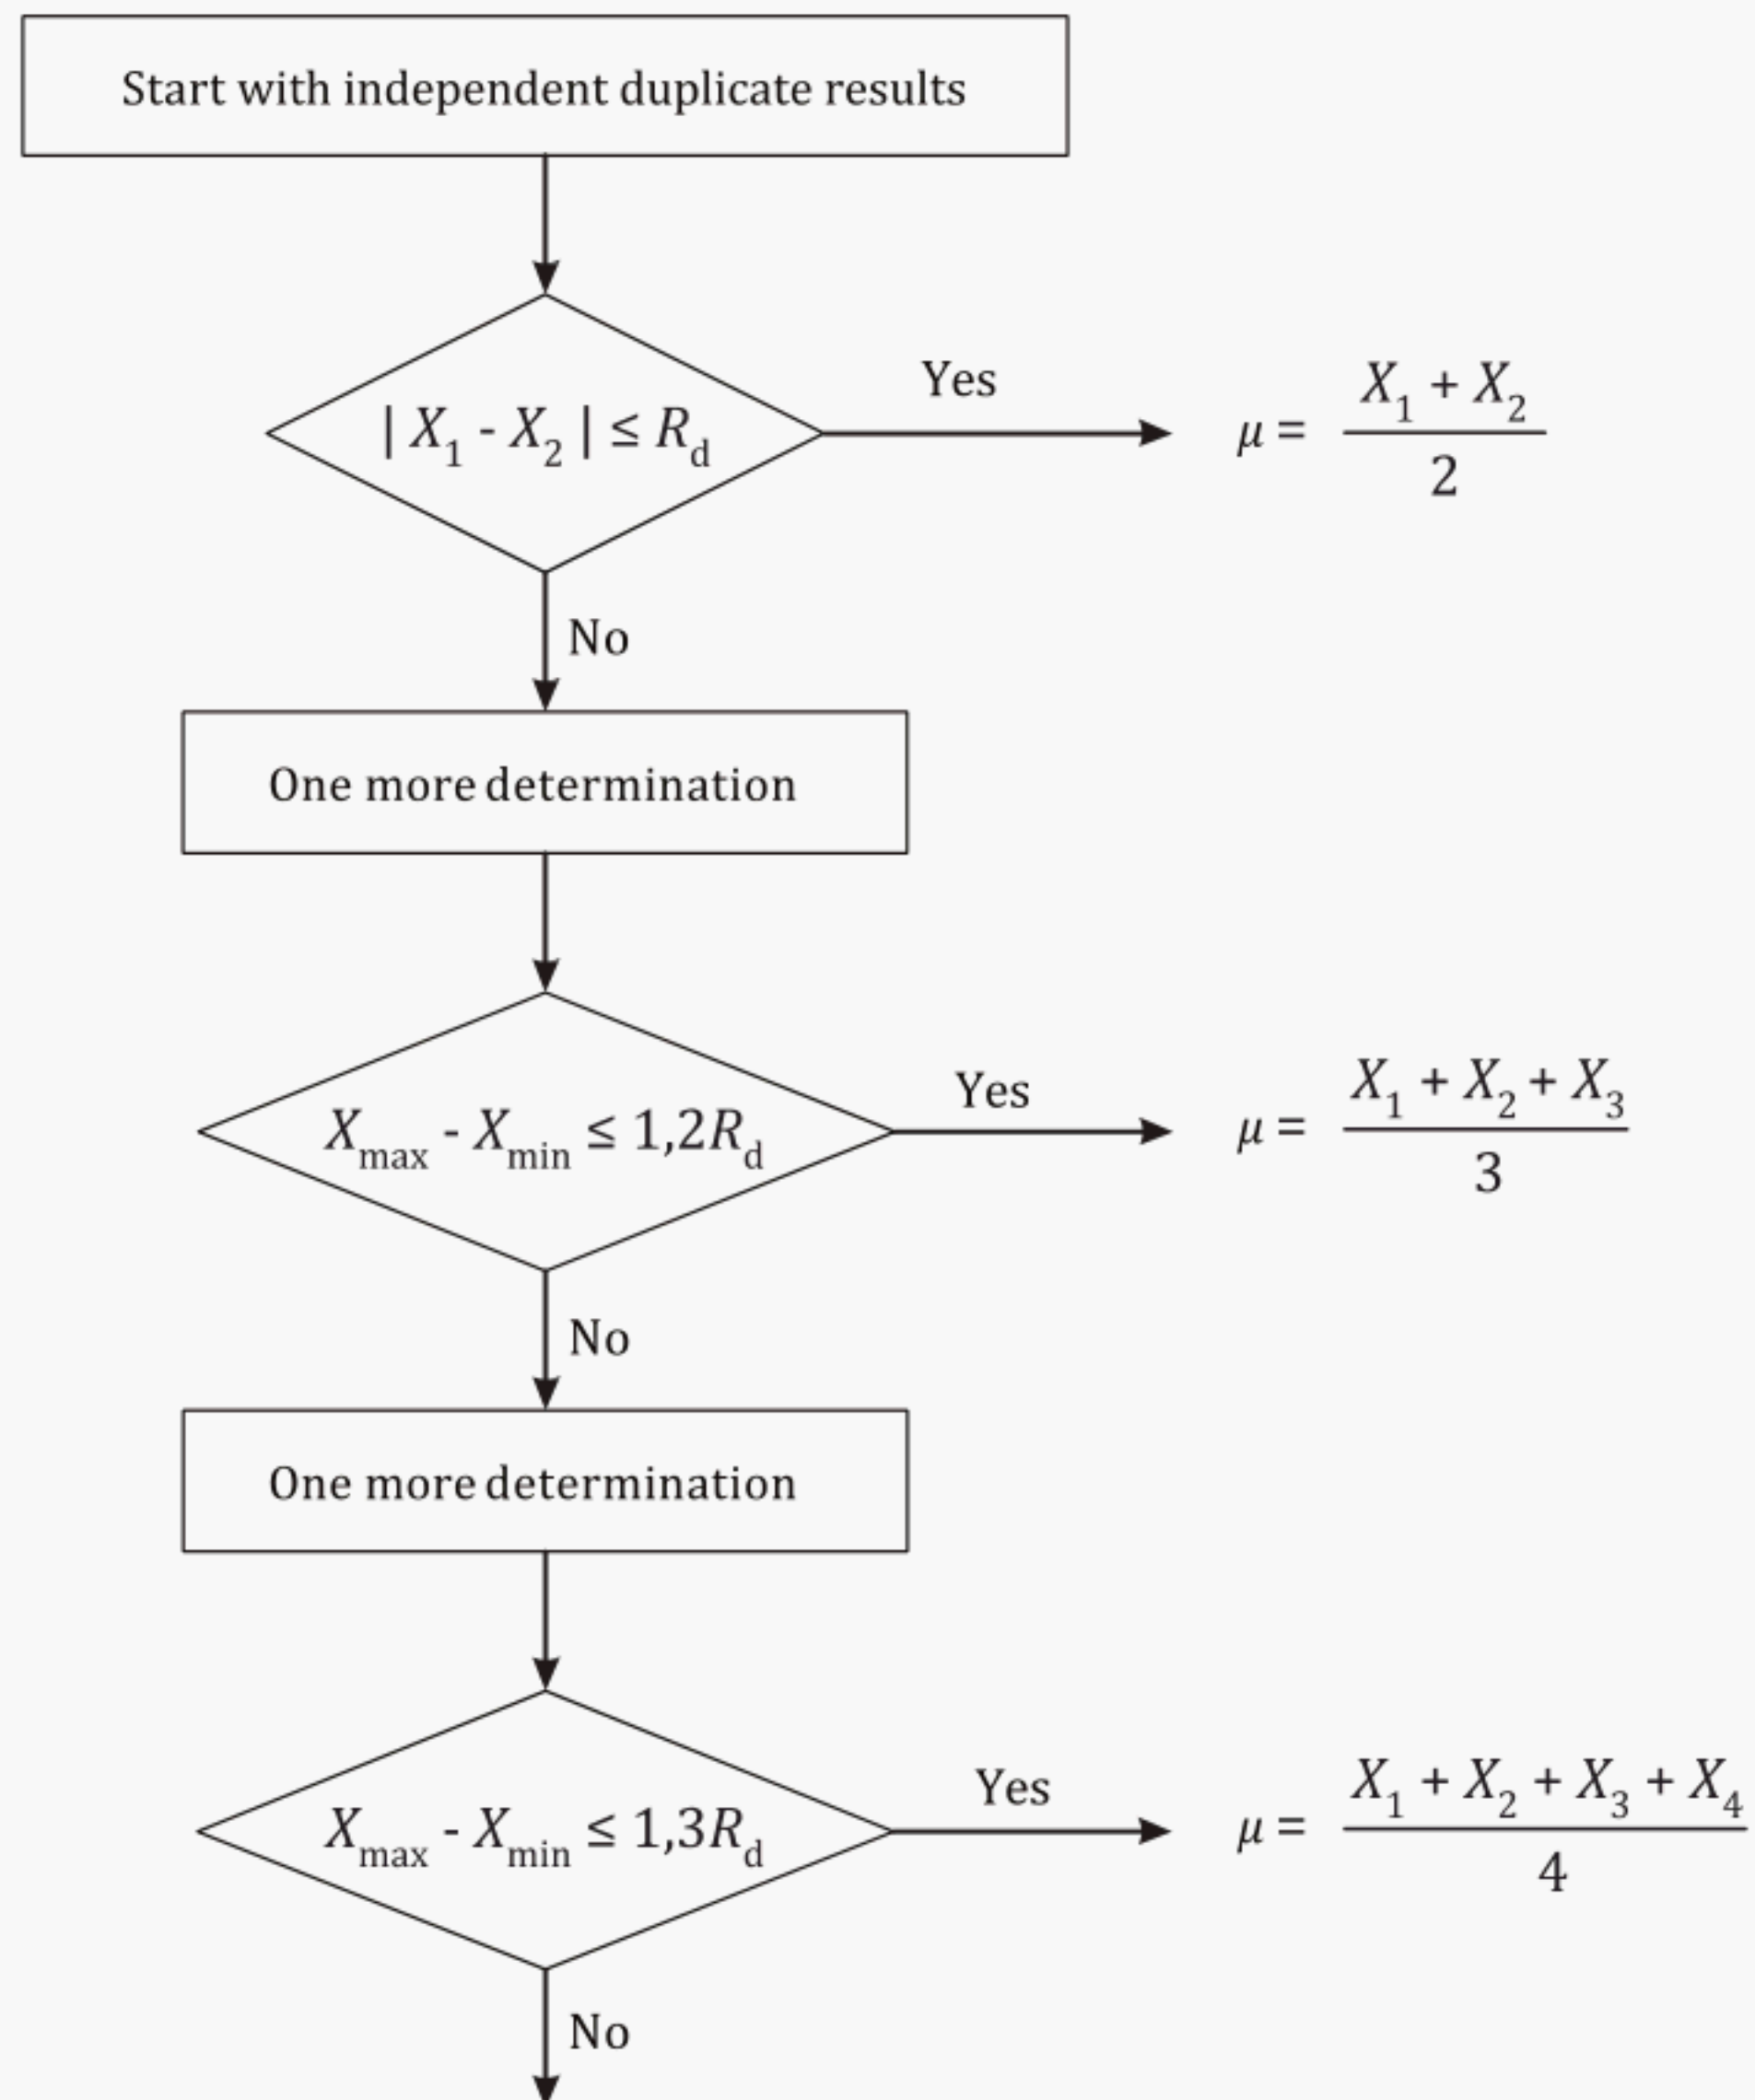

$$\mu = \text{Median } (X_1, X_2, X_3, X_4)$$

Where  $R_d = r$ ,  $r$  is given in [10.2](#).

## **Bibliography**

- [1] ISO 3696, *Water for analytical laboratory use — Specification and test methods*



**Standards Australia**

Standards Australia develops Australian Standards® and other documents of public benefit and national interest. These Standards are developed through an open process of consultation and consensus, in which all interested parties are invited to participate. Through a Memorandum of Understanding with the Commonwealth Government, Standards Australia is recognized as Australia's peak non-government national standards body.

For further information visit [www.standards.org.au](http://www.standards.org.au)

**Australian Standards®**

Committees of experts from industry, governments, consumers and other relevant sectors prepare Australian Standards. The requirements or recommendations contained in published Standards are a consensus of the views of representative interests and also take account of comments received from other sources. They reflect the latest scientific and industry experience. Australian Standards are kept under continuous review after publication and are updated regularly to take account of changing technology.

**International Involvement**

Standards Australia is responsible for ensuring the Australian viewpoint is considered in the formulation of International Standards and that the latest international experience is incorporated in national Standards. This role is vital in assisting local industry to compete in international markets. Standards Australia represents Australia at both the International Organization for Standardization (ISO) and the International Electrotechnical Commission (IEC).



GPO Box 476 Sydney NSW 2001  
Phone (02) 9237 6000  
[mail@standards.org.au](mailto:mail@standards.org.au)  
[www.standards.org.au](http://www.standards.org.au)



This page has been left intentionally blank.